


7470A

LB97147

INSTRUMENT ID: CV1

 μ Abs.:

38556

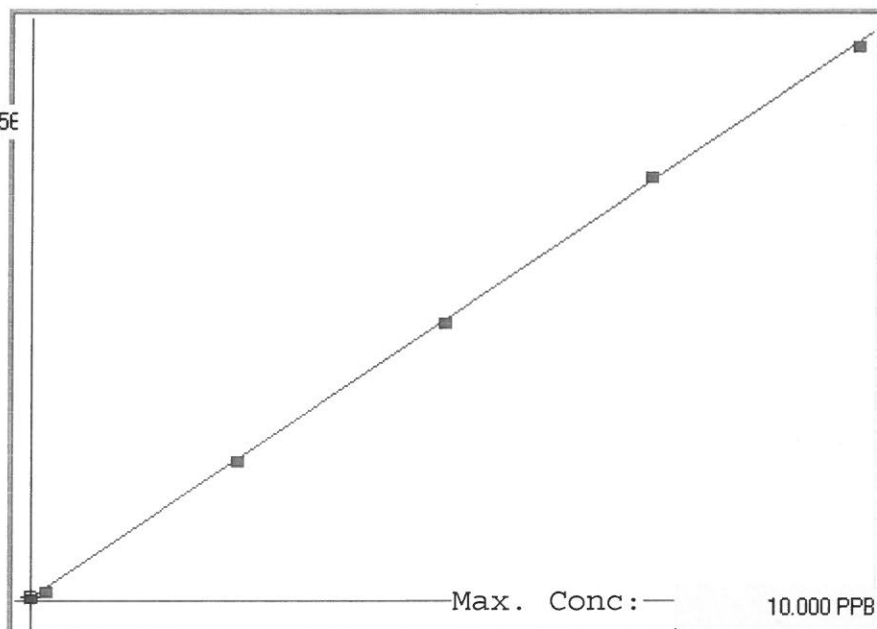

Linear

A= 0.0000e+000

B= 2.5865e-004

C= -3.6072e-002

Rho= 0.9998979

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.037	0.037	281	0.000	281				
0.2	0.200	0.151	-0.049	723	0.0 %	723				
2.5	2.500	2.494	-0.006	9783	0.0 %	9783				
5.0	5.000	4.988	-0.012	19424	0.0 %	19424				
7.5	7.500	7.593	0.093	29497	0.0 %	29497				
10.0	10.000	9.937	-0.063	38556	0.0 %	38556				

LB97147 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Aug 2018 10:09:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	281	-	0.0000	7470A	PPB	07 Aug 2018 10:37:06	S	Std
0.2 - 1	50.2	723	-	0.2000	7470A	PPB	07 Aug 2018 10:39:14	S	Std
2.5 - 1	52.5	9783	-	2.5000	7470A	PPB	07 Aug 2018 10:41:23	S	Std
5.0 - 1	55	19424	-	5.0000	7470A	PPB	07 Aug 2018 10:43:31	S	Std
7.5 - 1	57.5	29497	-	7.5000	7470A	PPB	07 Aug 2018 10:45:39	S	Std
10.0 - 1	510	38556	-	10.0000	7470A	PPB	07 Aug 2018 10:47:47	S	Std
ICV92 - 1	ICV92	16074	4.1215	-	7470A	PPB	07 Aug 2018 11:00:53	U	SMPL
ICB92 - 1	ICB92	326	0.0482	-	7470A	PPB	07 Aug 2018 11:02:59	U	SMPL
CCV17 - 1	CCV17	18928	4.8597	-	7470A	PPB	07 Aug 2018 11:05:07	U	SMPL
CCB17 - 1	CCB17	269	0.0335	-	7470A	PPB	07 Aug 2018 11:07:13	U	SMPL
CRA - 1	CRA	696	0.1440	-	7470A	PPB	07 Aug 2018 11:09:22	U	SMPL
HighStd - 1	HighStd	38587	9.9446	-	7470A	PPB	07 Aug 2018 11:11:29	U	SMPL
ChkStd - 1	ChkStd	26913	6.9251	-	7470A	PPB	07 Aug 2018 11:13:36	U	SMPL
PB111806BL - 1	PBW	283	0.0371	-	7470A	PPB	07 Aug 2018 11:15:45	U	SMPL
PB111806BS - 1	LCSW	14634	3.7491	-	7470A	PPB	07 Aug 2018 11:17:54	U	SMPL
PB111806TB - 1	PB111759TB	557	0.1080	-	7470A	PPB	07 Aug 2018 11:20:02	U	SMPL
J4277-02 - 1	OR-02-080318-A	619	0.1240	-	7470A	PPB	07 Aug 2018 11:22:10	U	SMPL
J4277-04 - 1	OR-02-080318-B	542	0.1041	-	7470A	PPB	07 Aug 2018 11:24:19	U	SMPL
J4283-02 - 1	TR-04-080318	618	0.1238	-	7470A	PPB	07 Aug 2018 11:26:27	U	SMPL
J4333-04 - 1	SOIL-1	691	0.1427	-	7470A	PPB	07 Aug 2018 11:28:34	U	SMPL
CCV18 - 1	CCV18	18699	4.8005	-	7470A	PPB	07 Aug 2018 11:30:41	U	SMPL
CCB18 - 1	CCB18	467	0.0847	-	7470A	PPB	07 Aug 2018 11:50:20	U	SMPL
J4333-04DUP - 1	SOIL-1DUP	752	0.1584	-	7470A	PPB	07 Aug 2018 11:52:26	U	SMPL
J4333-04MS - 1	SOIL-1MS	14368	3.6803	-	7470A	PPB	07 Aug 2018 11:54:32	U	SMPL
J4333-04MSD - 1	SOIL-1MSD	14011	3.5879	-	7470A	PPB	07 Aug 2018 11:56:39	U	SMPL
J4333-08 - 1	SOIL-2	738	0.1548	-	7470A	PPB	07 Aug 2018 11:58:46	U	SMPL
J4333-12 - 1	SOIL-3	1150	0.2614	-	7470A	PPB	07 Aug 2018 12:00:54	U	SMPL
J4333-16 - 1	SOIL-4	657	0.1339	-	7470A	PPB	07 Aug 2018 12:03:02	U	SMPL
J4333-20 - 1	SOIL-5	696	0.1440	-	7470A	PPB	07 Aug 2018 12:05:10	U	SMPL
J4333-23 - 1	OILY-DEBRIS	715	0.1489	-	7470A	PPB	07 Aug 2018 12:07:19	U	SMPL
J4335-03 - 1	CINNAMINSON-8-3-18	713	0.1483	-	7470A	PPB	07 Aug 2018 12:09:28	U	SMPL
J4345-03 - 1	RBR200035	737	0.1546	-	7470A	PPB	07 Aug 2018 12:11:35	U	SMPL
CCV19 - 1	CCV19	19019	4.8833	-	7470A	PPB	07 Aug 2018 12:13:42	U	SMPL
CCB19 - 1	CCB19	-147	-0.0741	-	7470A	PPB	07 Aug 2018 12:15:49	U	SMPL
J4347-05 - 1	CONCRETE-PILE-1	741	0.1556	-	7470A	PPB	07 Aug 2018 12:17:56	U	SMPL
J4348-05 - 1	72-11930	647	0.1313	-	7470A	PPB	07 Aug 2018 12:20:03	U	SMPL
J4349-01 - 1	NA-FILTER-BAGS	672	0.1377	-	7470A	PPB	07 Aug 2018 12:22:10	U	SMPL
J4355-02 - 1	WC-SOIL	507	0.0951	-	7470A	PPB	07 Aug 2018 12:24:17	U	SMPL
PB111807BL - 1	PBW	518	0.0979	-	7470A	PPB	07 Aug 2018 12:26:24	U	SMPL
PB111807BS - 1	LCSW	14177	3.6309	-	7470A	PPB	07 Aug 2018 12:28:31	U	SMPL
J4355-03 - 1	WC-WATER	449	0.0801	-	7470A	PPB	07 Aug 2018 12:30:39	U	SMPL
J4355-03DUP - 1	WC-WATERDUP	592	0.1171	-	7470A	PPB	07 Aug 2018 12:32:47	U	SMPL
J4355-03MS - 1	WC-WATERMS	14667	3.7576	-	7470A	PPB	07 Aug 2018 12:34:56	U	SMPL
J4355-03MSD - 1	WC-WATERMSD	13878	3.5535	-	7470A	PPB	07 Aug 2018 12:37:03	U	SMPL
CCV20 - 1	CCV20	19112	4.9073	-	7470A	PPB	07 Aug 2018 12:39:10	U	SMPL
CCB20 - 1	CCB20	413	0.0708	-	7470A	PPB	07 Aug 2018 12:41:17	U	SMPL
J4366-01 - 1	SV30518L	1379	0.3206	-	7470A	PPB	07 Aug 2018 12:43:25	U	SMPL
J4333-04LX5 - 1		92	-0.0123	-	7470A	PPB	07 Aug 2018 12:45:32	U	SMPL
J4333-04A - 1		15432	3.9555	-	7470A	PPB	07 Aug 2018 12:47:39	U	SMPL
J4355-03LX5 - 1		-86	-0.0583	-	7470A	PPB	07 Aug 2018 12:49:46	U	SMPL
J4355-03A - 1		15952	4.0900	-	7470A	PPB	07 Aug 2018 12:51:54	U	SMPL
CCV21 - 1	CCV21	18744	4.8121	-	7470A	PPB	07 Aug 2018 12:54:02	U	SMPL
CCB21 - 1	CCB21	-180	-0.0826	-	7470A	PPB	07 Aug 2018 12:56:11	U	SMPL