


7470A

LB 97168
INSTRUMENT ID: CYL

Linear

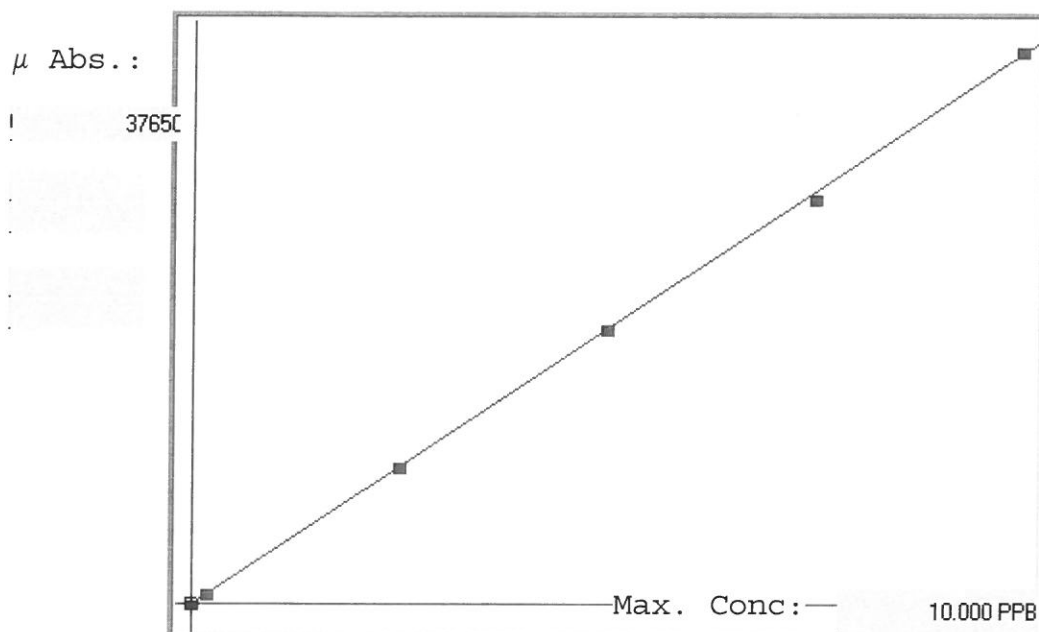

A= 0.0000e+000

B= 2.6730e-004

C= 1.7046e-002

Rho= 0.9998838

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.016	0.016	-3	0.000	-3				
0.2	0.200	0.217	0.017	748	0.0 %	748				
2.5	2.500	2.495	-0.005	9272	0.0 %	9272				
5.0	5.000	4.999	-0.001	18639	0.0 %	18639				
7.5	7.500	7.391	-0.109	27587	0.0 %	27587				
10.0	10.000	10.081	0.081	37650	0.0 %	37650				

LB97168

Method: 7470A

Operator: Admin

Date of Analysis: 08 Aug 2018 09:15:39

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-3	-	0.0000	7470A	PPB	08 Aug 2018 09:19:29	S	Std
0.2 - 1	50.2	748	-	0.2000	7470A	PPB	08 Aug 2018 09:21:37	S	Std
2.5 - 1	52.5	9272	-	2.5000	7470A	PPB	08 Aug 2018 09:23:45	S	Std
5.0 - 1	55	18639	-	5.0000	7470A	PPB	08 Aug 2018 09:25:53	S	Std
7.5 - 1	57.5	27587	-	7.5000	7470A	PPB	08 Aug 2018 09:28:01	S	Std
10.0 - 1	510	37650	-	10.0000	7470A	PPB	08 Aug 2018 09:32:33	S	Std
ICV95 - 1	ICV95	14298	3.8389	-	7470A	PPB	08 Aug 2018 09:35:09	U	SMPL
ICB95 - 1	ICB95	-268	-0.0546	-	7470A	PPB	08 Aug 2018 09:37:16	U	SMPL
CCV28 - 1	CCV28	18858	5.0578	-	7470A	PPB	08 Aug 2018 09:39:24	U	SMPL
CCB28 - 1	CCB28	-256	-0.0514	-	7470A	PPB	08 Aug 2018 09:41:31	U	SMPL
CRA - 1	CRA	723	0.2103	-	7470A	PPB	08 Aug 2018 09:43:38	U	SMPL
HighStd - 1	HighStd	37785	10.1170	-	7470A	PPB	08 Aug 2018 09:45:45	U	SMPL
ChkStd - 1	ChkStd	24780	6.6408	-	7470A	PPB	08 Aug 2018 09:47:52	U	SMPL
PB111861BL - 1	PBW	-195	-0.0351	-	7470A	PPB	08 Aug 2018 09:50:01	U	SMPL
PB111861BS - 1	LCSW	12916	3.4695	-	7470A	PPB	08 Aug 2018 09:52:10	U	SMPL
PB111861TB - 1	PB111812TB	-54	0.0026	-	7470A	PPB	08 Aug 2018 09:54:17	U	SMPL
J4360-03 - 1	155-SOIL	37	0.0269	-	7470A	PPB	08 Aug 2018 09:56:26	U	SMPL
J4360-03DUP - 1	155-SOILDUP	126	0.0507	-	7470A	PPB	08 Aug 2018 09:58:34	U	SMPL
J4360-03MS - 1	155-SOILMS	12913	3.4687	-	7470A	PPB	08 Aug 2018 10:00:43	U	SMPL
J4360-03MSD - 1	155-SOILMSD	13043	3.5035	-	7470A	PPB	08 Aug 2018 10:02:49	U	SMPL
CCV29 - 1	CCV29	18794	5.0407	-	7470A	PPB	08 Aug 2018 10:04:56	U	SMPL
CCB29 - 1	CCB29	-223	-0.0426	-	7470A	PPB	08 Aug 2018 10:07:04	U	SMPL
J4360-06 - 1	155-CONCRETE	64	0.0342	-	7470A	PPB	08 Aug 2018 10:09:12	U	SMPL
PB111862BL - 1	PBW	114	0.0475	-	7470A	PPB	08 Aug 2018 10:11:18	U	SMPL
PB111862BS - 1	LCSW	12601	3.3853	-	7470A	PPB	08 Aug 2018 10:13:25	U	SMPL
PB111862TB - 1	PB111814TB	-29	0.0093	-	7470A	PPB	08 Aug 2018 10:15:32	U	SMPL
J4366-02 - 1	SV30518L	93	0.0419	-	7470A	PPB	08 Aug 2018 10:17:40	U	SMPL
J4366-02DUP - 1	SV30518LDUP	-48	0.0042	-	7470A	PPB	08 Aug 2018 10:19:48	U	SMPL
J4366-02MS - 1	SV30518LMS	12803	3.4393	-	7470A	PPB	08 Aug 2018 10:21:56	U	SMPL
J4366-02MSD - 1	SV30518LMSD	12826	3.4455	-	7470A	PPB	08 Aug 2018 10:24:04	U	SMPL
CCV30 - 1	CCV30	18963	5.0859	-	7470A	PPB	08 Aug 2018 10:26:13	U	SMPL
CCB30 - 1	CCB30	-240	-0.0471	-	7470A	PPB	08 Aug 2018 10:28:20	U	SMPL
J4360-03LX5 - 1		-10	0.0144	-	7470A	PPB	08 Aug 2018 10:30:27	U	SMPL
J4360-03A - 1		14403	3.8670	-	7470A	PPB	08 Aug 2018 10:32:34	U	SMPL
J4366-02LX5 - 1		-177	-0.0303	-	7470A	PPB	08 Aug 2018 10:34:41	U	SMPL
J4366-02A - 1		14648	3.9325	-	7470A	PPB	08 Aug 2018 10:36:48	U	SMPL
CCV31 - 1	CCV31	19150	5.1359	-	7470A	PPB	08 Aug 2018 10:38:55	U	SMPL
CCB31 - 1	CCB31	-249	-0.0495	-	7470A	PPB	08 Aug 2018 10:41:03	U	SMPL