

2B97181

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

8/8/2018 15:17

Test: Total CN ug/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.571	0.0	0.096	
ICB1	0.292	0.0	0.004	
CCV1	239.368	0.0	0.231	
CCB1	0.217	0.0	0.004	
PB111882BL	-0.115	0.0	0.003	
PB111882BS	97.952	0.0	0.096	
J4360-04	0.480	0.0	0.004	
J4374-01	2.865	0.0	0.006	
J4374-01DUP	2.841	0.0	0.006	
J4374-01MS	40.028	0.0	0.042	
J4374-01MSD	39.827	0.0	0.041	
CCV2	253.984	0.0	0.244	
CCB2	0.180	0.0	0.004	

N	13
Mean	59.653
SD	90.3072
CV%	151.39

Aquakem v. 7.2AQ1

Results from time period:

Wed Aug 08 15:13:29 2018

Wed Aug 08 15:17:22 2018

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1619	µg/l	8/8/2018 9:54:38	
5.0PPBCN	A	Total CN	P	4.6533	µg/l	8/8/2018 9:54:39	
10PPBCN	A	Total CN	P	9.7021	µg/l	8/8/2018 9:54:40	
50PPBCN	A	Total CN	P	49.7132	µg/l	8/8/2018 9:54:41	
100PPBCN	A	Total CN	P	101.7126	µg/l	8/8/2018 9:54:42	
250PPBCN	A	Total CN	P	249.3705	µg/l	8/8/2018 9:54:43	
500PPBCN	A	Total CN	P	500.0103	µg/l	8/8/2018 9:54:44	
ICV1	S	Total CN	P	97.5711	µg/l	8/8/2018 15:13:29	
ICB1	S	Total CN	P	0.2917	µg/l	8/8/2018 15:13:30	
CCV1	S	Total CN	P	239.3683	µg/l	8/8/2018 15:13:31	
CCB1	S	Total CN	P	0.2169	µg/l	8/8/2018 15:13:32	
PB111882BL	S	Total CN	P	-0.1154	µg/l	8/8/2018 15:13:33	
PB111882BS	S	Total CN	P	97.9524	µg/l	8/8/2018 15:13:34	
J4360-04	S	Total CN	P	0.4798	µg/l	8/8/2018 15:13:35	
J4374-01	S	Total CN	P	2.8652	µg/l	8/8/2018 15:13:36	
J4374-01DUP	S	Total CN	P	2.841	µg/l	8/8/2018 15:13:37	
J4374-01MS	S	Total CN	P	40.0277	µg/l	8/8/2018 15:13:38	
J4374-01MSD	S	Total CN	P	39.8267	µg/l	8/8/2018 15:13:39	
CCV2	S	Total CN	P	253.9843	µg/l	8/8/2018 15:17:20	
CCB2	S	Total CN	P	0.1801	µg/l	8/8/2018 15:17:21	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

8/8/2018 10:24


Test Total CN

Accepted 8/8/2018 10:24

Factor 1054
Bias 0.004

Coeff. of det. 0.999982

Errors

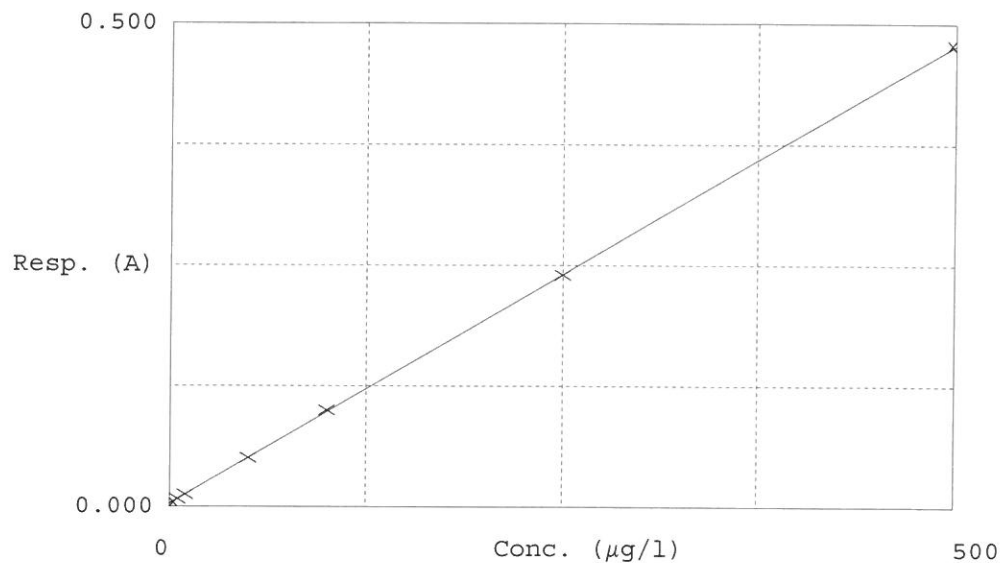

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.1619	0.0000	
2	5.0PPBCN	0.008	4.6533	5.0000	
3	10PPBCN	0.013	9.7021	10.0000	
4	50PPBCN	0.051	49.7132	50.0000	
5	100PPBCN	0.100	101.7126	100.0000	
6	250PPBCN	0.240	249.3705	250.0000	
7	500PPBCN	0.478	500.0103	500.0000	