

LB97191


7470A

INSTRUMENT ID: CVL

Linear

 μ Abs.:

40863

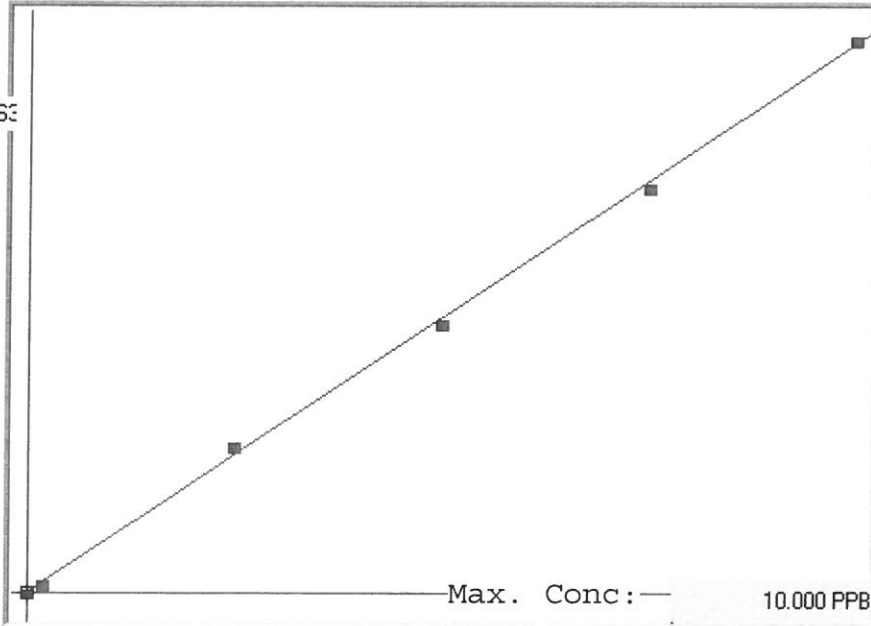

A= 0.0000e+000

B= 2.4690e-004

C= -8.0039e-003

Rho= 0.9996137

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.017	-0.017	-36	0.000	-36				
0.2	0.200	0.161	-0.039	684	0.0 %	684				
2.5	2.500	2.682	0.182	10894	0.0 %	10894				
5.0	5.000	4.908	-0.092	19910	0.0 %	19910				
7.5	7.500	7.385	-0.115	29944	0.0 %	29944				
10.0	10.000	10.081	0.081	40863	0.0 %	40863				

LB97191 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 09 Aug 2018 09:52:49

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-36	-	0.00007470A	PPB		09 Aug 2018 09:58:27	S	Std
0.2 - 1	50.2	684	-	0.20007470A	PPB		09 Aug 2018 10:00:35	S	Std
2.5 - 1	52.5	10894	-	2.50007470A	PPB		09 Aug 2018 10:02:44	S	Std
5.0 - 1	55	19910	-	5.00007470A	PPB		09 Aug 2018 10:07:43	S	Std
7.5 - 1	57.5	29944	-	7.50007470A	PPB		09 Aug 2018 10:12:17	S	Std
10.0 - 1	57.5	40863	-	10.00007470A	PPB		09 Aug 2018 10:16:49	S	Std
ICV98 - 1	ICV98	14462	3.8828	-7470A	PPB		09 Aug 2018 10:19:18	U	SMPL
ICB98 - 1	ICB98	-235	-0.0458	-7470A	PPB		09 Aug 2018 10:21:26	U	SMPL
CCV38 - 1	CCV38	20216	5.4208	-7470A	PPB		09 Aug 2018 10:23:33	U	SMPL
CCB38 - 1	CCB38	-228	-0.0439	-7470A	PPB		09 Aug 2018 10:25:39	U	SMPL
CRA - 1	CRA	782	0.2261	-7470A	PPB		09 Aug 2018 10:27:47	U	SMPL
HighStd - 1	HighStd	37067	9.9251	-7470A	PPB		09 Aug 2018 10:32:26	U	SMPL
ChkStd - 1	ChkStd	25495	6.8319	-7470A	PPB		09 Aug 2018 10:34:32	U	SMPL
PB111873BL - 1	PBW	-92	-0.0307	-7470A	PPB		09 Aug 2018 10:39:08	U	SMPL
PB111873BS - 1	LCSW	13808	3.4012	-7470A	PPB		09 Aug 2018 10:41:15	U	SMPL
PB111873TB - 1	PB111845TB	-201	-0.0576	-7470A	PPB		09 Aug 2018 10:43:23	U	SMPL
J4275-02 - 1	CL-02-080718-A	-95	-0.0315	-7470A	PPB		09 Aug 2018 10:45:31	U	SMPL
J4275-02DUP - 1	CL-02-080718-ADUP	-48	-0.0199	-7470A	PPB		09 Aug 2018 10:47:39	U	SMPL
J4275-02MS - 1	CL-02-080718-AMS	13988	3.4457	-7470A	PPB		09 Aug 2018 10:49:47	U	SMPL
J4275-02MSD - 1	CL-02-080718-AMSD	13932	3.4318	-7470A	PPB		09 Aug 2018 10:51:54	U	SMPL
CCV39 - 1	CCV39	20404	5.0298	-7470A	PPB		09 Aug 2018 10:57:32	U	SMPL
CCB39 - 1	CCB39	-219	-0.0621	-7470A	PPB		09 Aug 2018 10:59:39	U	SMPL
J4275-04 - 1	CL-02-080718-B	-78	-0.0273	-7470A	PPB		09 Aug 2018 11:01:46	U	SMPL
J4275-06 - 1	CL-02-080718-C	-47	-0.0196	-7470A	PPB		09 Aug 2018 11:03:52	U	SMPL
J4275-08 - 1	CL-02-080718-D	-60	-0.0228	-7470A	PPB		09 Aug 2018 11:05:59	U	SMPL
J4276-02 - 1	OK-02-080718	-39	-0.0176	-7470A	PPB		09 Aug 2018 11:08:06	U	SMPL
J4375-02 - 1	OILY-DEBRIS-DRUM-A	509	0.1177	-7470A	PPB		09 Aug 2018 11:10:13	U	SMPL
J4375-04 - 1	OILY-DEBRIS-DRUM-B	-142	-0.0431	-7470A	PPB		09 Aug 2018 11:12:21	U	SMPL
PB111874BL - 1	PBW	-33	-0.0162	-7470A	PPB		09 Aug 2018 11:14:29	U	SMPL
PB111874BS - 1	LCSW	14098	3.4728	-7470A	PPB		09 Aug 2018 11:16:38	U	SMPL
PB111874TB - 1	PB111847TB	-166	-0.0490	-7470A	PPB		09 Aug 2018 11:18:46	U	SMPL
J4374-02 - 1	OILY-WATER	-57	-0.0221	-7470A	PPB		09 Aug 2018 11:20:53	U	SMPL
CCV40 - 1	CCV40	20049	4.9421	-7470A	PPB		09 Aug 2018 11:23:00	U	SMPL
CCB40 - 1	CCB40	-223	-0.0631	-7470A	PPB		09 Aug 2018 11:25:07	U	SMPL
J4374-02DUP - 1	OILY-WATERDUP	-90	-0.0302	-7470A	PPB		09 Aug 2018 11:27:15	U	SMPL
J4374-02MS - 1	OILY-WATERMS	14786	3.6427	-7470A	PPB		09 Aug 2018 11:29:22	U	SMPL
J4374-02MSD - 1	OILY-WATERMSD	14324	3.5286	-7470A	PPB		09 Aug 2018 11:31:28	U	SMPL
PB111875BL - 1	PBW	-216	-0.0613	-7470A	PPB		09 Aug 2018 11:33:36	U	SMPL
PB111875BS - 1	LCSW	13877	3.4183	-7470A	PPB		09 Aug 2018 11:35:45	U	SMPL
J4374-01 - 1	OILY-WATER	1124	0.2695	-7470A	PPB		09 Aug 2018 11:37:52	U	SMPL
J4379-01 - 1	FB-08072018	-242	-0.0678	-7470A	PPB		09 Aug 2018 11:40:00	U	SMPL
J4379-03 - 1	MW-106S	-96	-0.0317	-7470A	PPB		09 Aug 2018 11:42:09	U	SMPL
J4379-04 - 1	MW-106I	-74	-0.0263	-7470A	PPB		09 Aug 2018 11:44:17	U	SMPL
J4379-05 - 1	MW-107S	-88	-0.0297	-7470A	PPB		09 Aug 2018 11:46:24	U	SMPL
CCV41 - 1	CCV41	19787	4.8775	-7470A	PPB		09 Aug 2018 11:48:31	U	SMPL
CCB41 - 1	CCB41	-209	-0.0596	-7470A	PPB		09 Aug 2018 11:50:38	U	SMPL
J4379-05DUP - 1	MW-107SDUP	-111	-0.0354	-7470A	PPB		09 Aug 2018 11:52:46	U	SMPL
J4379-05MS - 1	MW-107SMS	15322	3.7750	-7470A	PPB		09 Aug 2018 11:54:53	U	SMPL
J4379-05MSD - 1	MW-107SMSD	15005	3.6968	-7470A	PPB		09 Aug 2018 11:57:00	U	SMPL
J4383-01 - 1	JTY-GW-05	14923	3.6765	-7470A	PPB		09 Aug 2018 11:59:08	U	SMPL
J4275-02LX5 - 1		-313	-0.0853	-7470A	PPB		09 Aug 2018 12:01:15	U	SMPL
J4275-02A - 1		14023	3.4543	-7470A	PPB		09 Aug 2018 12:03:25	U	SMPL
J4374-02LX5 - 1		-137	-0.0418	-7470A	PPB		09 Aug 2018 12:05:33	U	SMPL
J4374-02A - 1		14354	3.5360	-7470A	PPB		09 Aug 2018 12:07:42	U	SMPL
J4379-05LX5 - 1		-134	-0.0411	-7470A	PPB		09 Aug 2018 12:09:50	U	SMPL
J4379-05A - 1		16468	4.0580	-7470A	PPB		09 Aug 2018 12:11:57	U	SMPL
CCV42 - 1	CCV42	19226	4.7389	-7470A	PPB		09 Aug 2018 12:14:04	U	SMPL
CCB42 - 1	CCB42	-198	-0.0569	-7470A	PPB		09 Aug 2018 12:16:11	U	SMPL