


7470A

LB97275
INSTRUMENT ID: CV1

Linear

 μ Abs.:

37315

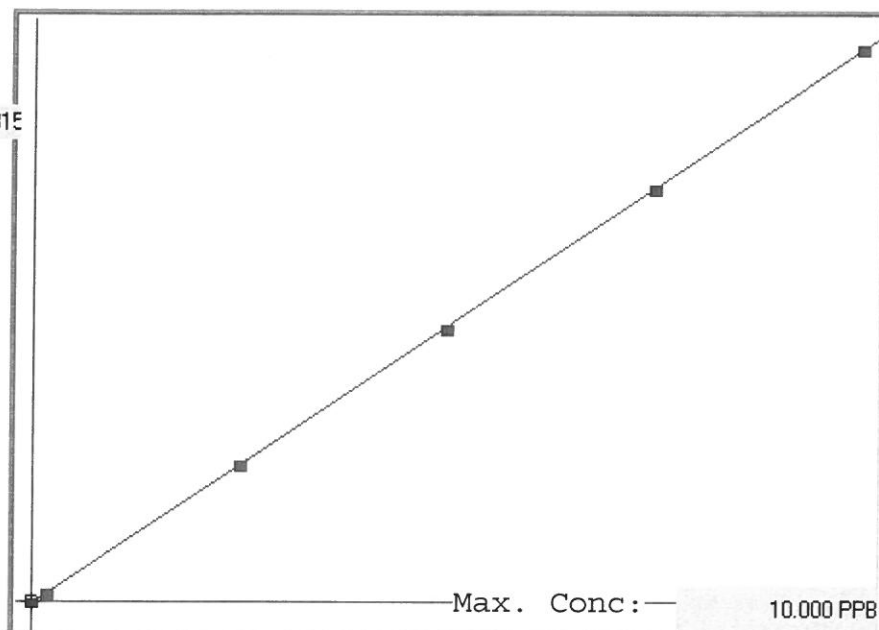

A= 0.0000e+000

B= 2.6756e-004

C= 3.6976e-002

Rho= 0.9999871

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	-87	0.000	-87				
0.2	0.200	0.203	0.003	621	0.0 %	621				
2.5	2.500	2.505	0.005	9223	0.0 %	9223				
5.0	5.000	4.962	-0.038	18408	0.0 %	18408				
7.5	7.500	7.495	-0.005	27875	0.0 %	27875				
10.0	10.000	10.021	0.021	37315	0.0 %	37315				

LB97275 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Aug 2018 11:06:48

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-87	-	0.0000	7470A	PPB	14 Aug 2018 11:37:12	S	Std
0.2 - 1	50.2	621	-	0.2000	7470A	PPB	14 Aug 2018 11:39:21	S	Std
2.5 - 1	52.5	9223	-	2.5000	7470A	PPB	14 Aug 2018 11:41:29	S	Std
5.0 - 1	55	18408	-	5.0000	7470A	PPB	14 Aug 2018 11:43:37	S	Std
7.5 - 1	57.5	27875	-	7.5000	7470A	PPB	14 Aug 2018 11:45:45	S	Std
10.0 - 1	510	37315	-	10.0000	7470A	PPB	14 Aug 2018 11:47:53	S	Std
ICV06 - 1	ICV06	14421	3.8955	-	7470A	PPB	14 Aug 2018 11:50:56	U	SMPL
ICB06 - 1	ICB06	-239	-0.0270	-	7470A	PPB	14 Aug 2018 11:53:02	U	SMPL
CCV73 - 1	CCV73	17413	4.6960	-	7470A	PPB	14 Aug 2018 11:55:09	U	SMPL
CCB73 - 1	CCB73	-229	-0.0243	-	7470A	PPB	14 Aug 2018 11:57:15	U	SMPL
CRA - 1	CRA	607	0.1994	-	7470A	PPB	14 Aug 2018 11:59:24	U	SMPL
HighStd - 1	HighStd	37399	10.0435	-	7470A	PPB	14 Aug 2018 12:01:30	U	SMPL
ChkStd - 1	ChkStd	26517	7.1319	-	7470A	PPB	14 Aug 2018 12:03:37	U	SMPL
PB111992BL - 1	PBW	-324	-0.0497	-	7470A	PPB	14 Aug 2018 12:05:45	U	SMPL
PB111992BS - 1	LCSW	13726	3.7095	-	7470A	PPB	14 Aug 2018 12:07:54	U	SMPL
PB111992TB - 1	PB111960TB	-184	-0.0123	-	7470A	PPB	14 Aug 2018 12:10:02	U	SMPL
J4423-02 - 1	72-11944	-79	0.0158	-	7470A	PPB	14 Aug 2018 12:12:10	U	SMPL
J4427-03 - 1	RB47197	-83	0.0148	-	7470A	PPB	14 Aug 2018 12:14:19	U	SMPL
J4442-10 - 1	SP-1-1	-49	0.0239	-	7470A	PPB	14 Aug 2018 12:16:28	U	SMPL
J4442-20 - 1	SP-1-2	-51	0.0233	-	7470A	PPB	14 Aug 2018 12:18:34	U	SMPL
CCV74 - 1	CCV74	18064	4.8702	-	7470A	PPB	14 Aug 2018 12:20:41	U	SMPL
CCB74 - 1	CCB74	-211	-0.0195	-	7470A	PPB	14 Aug 2018 12:22:48	U	SMPL
J4442-30 - 1	SP-1-3	-63	0.0201	-	7470A	PPB	14 Aug 2018 12:24:57	U	SMPL
J4442-40 - 1	SP-1-4	-31	0.0287	-	7470A	PPB	14 Aug 2018 12:27:04	U	SMPL
J4442-50 - 1	SP-1-5	6	0.0386	-	7470A	PPB	14 Aug 2018 12:29:10	U	SMPL
J4443-10 - 1	SALEM-RD-SP	-58	0.0215	-	7470A	PPB	14 Aug 2018 12:31:17	U	SMPL
J4447-05 - 1	SP-1-6	-50	0.0236	-	7470A	PPB	14 Aug 2018 12:33:25	U	SMPL
J4447-15 - 1	SP-1-7	-25	0.0303	-	7470A	PPB	14 Aug 2018 12:35:32	U	SMPL
J4447-25 - 1	SP-1-8	-35	0.0276	-	7470A	PPB	14 Aug 2018 12:37:40	U	SMPL
J4447-35 - 1	SP-1-9	-60	0.0209	-	7470A	PPB	14 Aug 2018 12:39:49	U	SMPL
J4447-45 - 1	SP-1-10	-29	0.0292	-	7470A	PPB	14 Aug 2018 12:41:57	U	SMPL
J4447-45DUP - 1	SP-1-10DUP	-36	0.0273	-	7470A	PPB	14 Aug 2018 12:44:04	U	SMPL
CCV75 - 1	CCV75	18057	4.8683	-	7470A	PPB	14 Aug 2018 12:46:11	U	SMPL
CCB75 - 1	CCB75	-206	-0.0181	-	7470A	PPB	14 Aug 2018 12:48:18	U	SMPL
J4447-45MS - 1	SP-1-10MS	13636	3.6854	-	7470A	PPB	14 Aug 2018 12:50:26	U	SMPL
J4447-45MSD - 1	SP-1-10MSD	14496	3.9155	-	7470A	PPB	14 Aug 2018 12:52:33	U	SMPL
PB111993BL - 1	PBW	-242	-0.0278	-	7470A	PPB	14 Aug 2018 12:54:40	U	SMPL
PB111993BS - 1	LCSW	13125	3.5487	-	7470A	PPB	14 Aug 2018 12:56:47	U	SMPL
PB111993TB - 1	PB111969TB	-207	-0.0184	-	7470A	PPB	14 Aug 2018 12:58:55	U	SMPL
J4449-03 - 1	TILCON-MH-001	261	0.1068	-	7470A	PPB	14 Aug 2018 13:05:39	U	SMPL
J4449-03DUP - 1	TILCON-MH-001DUP	111	0.0667	-	7470A	PPB	14 Aug 2018 13:07:46	U	SMPL
J4449-03MS - 1	TILCON-MH-001MS	13224	3.5752	-	7470A	PPB	14 Aug 2018 13:09:54	U	SMPL
J4449-03MSD - 1	TILCON-MH-001MSD	13628	3.6833	-	7470A	PPB	14 Aug 2018 13:12:03	U	SMPL
J4449-04 - 1	TILCON-PL-001	176	0.0841	-	7470A	PPB	14 Aug 2018 13:14:11	U	SMPL
CCV76 - 1	CCV76	18006	4.8547	-	7470A	PPB	14 Aug 2018 13:16:20	U	SMPL
CCB76 - 1	CCB76	-152	-0.0037	-	7470A	PPB	14 Aug 2018 13:18:28	U	SMPL
J4447-45LX5 - 1		-28	0.0295	-	7470A	PPB	14 Aug 2018 13:20:36	U	SMPL
J4447-45A - 1		13880	3.7507	-	7470A	PPB	14 Aug 2018 13:22:44	U	SMPL
J4449-03LX5 - 1		73	0.0565	-	7470A	PPB	14 Aug 2018 13:24:51	U	SMPL
J4449-03A - 1		14001	3.7831	-	7470A	PPB	14 Aug 2018 13:26:58	U	SMPL
CCV77 - 1	CCV77	17971	4.8453	-	7470A	PPB	14 Aug 2018 13:29:05	U	SMPL
CCB77 - 1	CCB77	-172	-0.0090	-	7470A	PPB	14 Aug 2018 13:31:14	U	SMPL