


7470A

L399333
INSTRUMENT ID: CV1

Linear

 μ Abs.:

35947

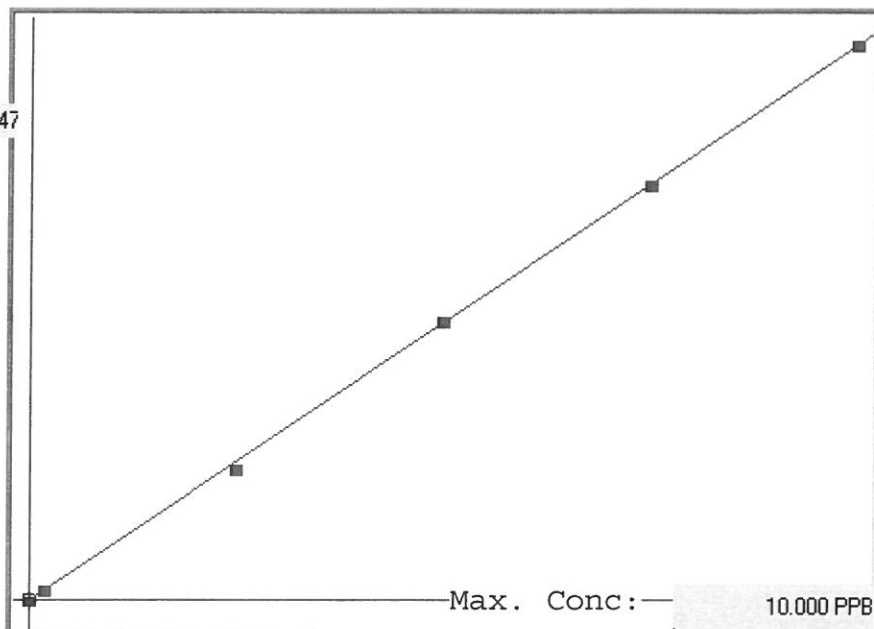

A= 0.0000e+000

B= 2.7758e-004

C= 2.2531e-002

Rho= 0.9999006

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.049	0.049	97	0.000	97				
0.2	0.200	0.205	0.005	657	0.0 %	657				
2.5	2.500	2.396	-0.104	8549	0.0 %	8549				
5.0	5.000	5.053	0.053	18124	0.0 %	18124				
7.5	7.500	7.496	-0.004	26924	0.0 %	26924				
10.0	10.000	10.001	0.001	35947	0.0 %	35947				

LB97333 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Aug 2018 09:49:09

Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	97	-	0.00007470A	PPB	16 Aug 2018 09:58:51	S	Std
0.2 - 1	50.2	657	-	0.20007470A	PPB	16 Aug 2018 10:00:59	S	Std
2.5 - 1	52.5	8549	-	2.50007470A	PPB	16 Aug 2018 10:03:07	S	Std
5.0 - 1	55	18124	-	5.00007470A	PPB	16 Aug 2018 10:05:15	S	Std
7.5 - 1	57.5	26924	-	7.50007470A	PPB	16 Aug 2018 10:07:23	S	Std
10.0 - 1	510	35947	-	10.00007470A	PPB	16 Aug 2018 10:09:31	S	Std
ICV11 - 1	ICV11	13980	3.9031	-7470A	PPB	16 Aug 2018 10:12:00	U	SMPL
ICB11 - 1	ICB11	-184	-0.0285	-7470A	PPB	16 Aug 2018 10:14:07	U	SMPL
CCV97 - 1	CCV97	18838	5.2516	-7470A	PPB	16 Aug 2018 10:16:16	U	SMPL
CCB97 - 1	CCB97	-207	-0.0349	-7470A	PPB	16 Aug 2018 10:18:22	U	SMPL
CRA - 1	CRA	605	0.1905	-7470A	PPB	16 Aug 2018 10:20:29	U	SMPL
HighStd - 1	HighStd	36598	10.1814	-7470A	PPB	16 Aug 2018 10:22:36	U	SMPL
ChkStd - 1	ChkStd	24693	6.8768	-7470A	PPB	16 Aug 2018 10:24:43	U	SMPL
PB112093BL - 1	PBW	-258	-0.0491	-7470A	PPB	16 Aug 2018 10:26:52	U	SMPL
PB112093BS - 1	LCSW	13293	3.7124	-7470A	PPB	16 Aug 2018 10:29:02	U	SMPL
PB112093TB - 1	PB112054TB	-130	-0.0136	-7470A	PPB	16 Aug 2018 10:31:09	U	SMPL
J4471-04 - 1	TP-1	-15	0.0184	-7470A	PPB	16 Aug 2018 10:33:18	U	SMPL
J4471-04DUP - 1	TP-1DUP	3	0.0234	-7470A	PPB	16 Aug 2018 10:35:26	U	SMPL
J4471-04MS - 1	TP-1MS	13338	3.7249	-7470A	PPB	16 Aug 2018 10:37:35	U	SMPL
J4471-04MSD - 1	TP-1MSD	13648	3.8109	-7470A	PPB	16 Aug 2018 10:39:41	U	SMPL
CCV98 - 1	CCV98	18552	5.1722	-7470A	PPB	16 Aug 2018 10:41:48	U	SMPL
CCB98 - 1	CCB98	-162	-0.0224	-7470A	PPB	16 Aug 2018 10:43:55	U	SMPL
J4471-08 - 1	TP-2	-17	0.0178	-7470A	PPB	16 Aug 2018 10:46:03	U	SMPL
J4471-12 - 1	TP-3	9	0.0250	-7470A	PPB	16 Aug 2018 10:48:10	U	SMPL
J4471-16 - 1	TP-4	21	0.0284	-7470A	PPB	16 Aug 2018 10:50:16	U	SMPL
J4471-20 - 1	TP-5	43	0.0345	-7470A	PPB	16 Aug 2018 10:52:23	U	SMPL
J4471-24 - 1	TP-6	36	0.0325	-7470A	PPB	16 Aug 2018 10:54:31	U	SMPL
J4471-27 - 1	BED-ROCK	19	0.0278	-7470A	PPB	16 Aug 2018 10:56:38	U	SMPL
PB112094BL - 1	PBW	15	0.0267	-7470A	PPB	16 Aug 2018 10:58:47	U	SMPL
PB112094BS - 1	LCSW	12981	3.6258	-7470A	PPB	16 Aug 2018 11:00:55	U	SMPL
PB112094TB - 1	PB112056TB	-103	-0.0061	-7470A	PPB	16 Aug 2018 11:03:04	U	SMPL
J4474-02 - 1	FRAC-TANK-SV28570L	-10	0.0198	-7470A	PPB	16 Aug 2018 11:05:11	U	SMPL
CCV99 - 1	CCV99	18417	5.1347	-7470A	PPB	16 Aug 2018 11:07:18	U	SMPL
CCB99 - 1	CCB99	-175	-0.0260	-7470A	PPB	16 Aug 2018 11:09:25	U	SMPL
J4474-02DUP - 1	FRAC-TANK-SV28570LDUP	0	0.0225	-7470A	PPB	16 Aug 2018 11:11:33	U	SMPL
J4474-02MS - 1	FRAC-TANK-SV28570LMS	13165	3.6769	-7470A	PPB	16 Aug 2018 11:13:40	U	SMPL
J4474-02MSD - 1	FRAC-TANK-SV28570LMSD	13350	3.7282	-7470A	PPB	16 Aug 2018 11:15:47	U	SMPL
PB112095BL - 1	PBW	-134	-0.0147	-7470A	PPB	16 Aug 2018 11:17:55	U	SMPL
PB112095BS - 1	LCSW	13525	3.7768	-7470A	PPB	16 Aug 2018 11:20:03	U	SMPL
J4474-01 - 1	FRAC-TANK-SV28570L	826	0.2518	-7470A	PPB	16 Aug 2018 11:26:51	U	SMPL
J4474-01DUP - 1	FRAC-TANK-SV28570LDUP	769	0.2360	-7470A	PPB	16 Aug 2018 11:28:59	U	SMPL
J4474-01MS - 1	FRAC-TANK-SV28570LMS	14103	3.9372	-7470A	PPB	16 Aug 2018 11:31:07	U	SMPL
J4474-01MSD - 1	FRAC-TANK-SV28570LMSD	13964	3.8986	-7470A	PPB	16 Aug 2018 11:35:42	U	SMPL
J4494-01 - 1	FL-0565	-109	-0.0077	-7470A	PPB	16 Aug 2018 11:37:48	U	SMPL
CCV01 - 1	CCV01	18161	5.0636	-7470A	PPB	16 Aug 2018 11:39:57	U	SMPL
CCB01 - 1	CCB01	-110	-0.0080	-7470A	PPB	16 Aug 2018 11:42:04	U	SMPL
J4502-03 - 1	BROWN-FRAC-TANK	2474	0.7093	-7470A	PPB	16 Aug 2018 11:44:12	U	SMPL
J4471-04LX5 - 1		-117	-0.0099	-7470A	PPB	16 Aug 2018 11:46:19	U	SMPL
J4471-04A - 1		13992	3.9064	-7470A	PPB	16 Aug 2018 11:53:14	U	SMPL
J4474-02LX5 - 1		-205	-0.0344	-7470A	PPB	16 Aug 2018 11:55:21	U	SMPL
J4474-02A - 1		14213	3.9678	-7470A	PPB	16 Aug 2018 11:57:30	U	SMPL
J4474-01LX5 - 1		29	0.0306	-7470A	PPB	16 Aug 2018 11:59:37	U	SMPL
J4474-01A - 1		14998	4.1857	-7470A	PPB	16 Aug 2018 12:01:46	U	SMPL
CCV02 - 1	CCV02	18137	5.0570	-7470A	PPB	16 Aug 2018 12:03:54	U	SMPL
CCB02 - 1	CCB02	-101	-0.0055	-7470A	PPB	16 Aug 2018 12:06:04	U	SMPL