


7470A

LB 97365
INSTRUMENT ID: CV1

Linear

 μ Abs.:

36233

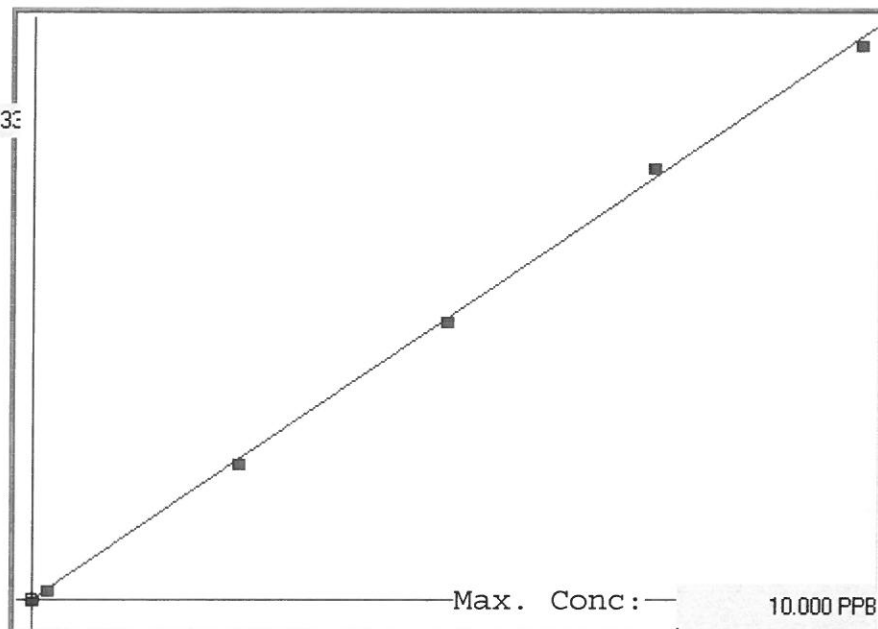

A= 0.0000e+000

B= 2.7233e-004

C= 5.0324e-003

Rho= 0.9996172

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.015	0.015	36	0.000	36				
0.2	0.200	0.199	-0.001	713	0.0 %	713				
2.5	2.500	2.446	-0.054	8963	0.0 %	8963				
5.0	5.000	4.963	-0.037	18207	0.0 %	18207				
7.5	7.500	7.704	0.204	28272	0.0 %	28272				
10.0	10.000	9.872	-0.128	36233	0.0 %	36233				

LB97365 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Aug 2018 10:48:09

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	36	-	0.0000	7470A	PPB	17 Aug 2018 10:49:25	S	Std
0.2 - 1	50.2	713	-	0.2000	7470A	PPB	17 Aug 2018 10:51:34	S	Std
2.5 - 1	52.5	8963	-	2.5000	7470A	PPB	17 Aug 2018 10:53:42	S	Std
5.0 - 1	53	18207	-	5.0000	7470A	PPB	17 Aug 2018 10:55:50	S	Std
7.5 - 1	57.5	28272	-	7.5000	7470A	PPB	17 Aug 2018 10:57:58	S	Std
10.0 - 1	518	36233	-	10.0000	7470A	PPB	17 Aug 2018 11:00:06	S	Std
ICV14 - 1	ICV14	14371	3.9187	-	7470A	PPB	17 Aug 2018 11:02:51	U	SMPL
ICB14 - 1	ICB14	-182	-0.0445	-	7470A	PPB	17 Aug 2018 11:04:57	U	SMPL
CCV12 - 1	CCV12	18008	4.9091	-	7470A	PPB	17 Aug 2018 11:09:27	U	SMPL
CCB12 - 1	CCB12	-197	-0.0486	-	7470A	PPB	17 Aug 2018 11:11:34	U	SMPL
CRA - 1	CRA	655	0.1834	-	7470A	PPB	17 Aug 2018 11:13:41	U	SMPL
HighStd - 1	HighStd	36108	9.8383	-	7470A	PPB	17 Aug 2018 11:15:48	U	SMPL
ChkStd - 1	ChkStd	25422	6.9282	-	7470A	PPB	17 Aug 2018 11:17:55	U	SMPL
PB112135BL - 1	PBW	-294	-0.0750	-	7470A	PPB	17 Aug 2018 11:20:04	U	SMPL
PB112135BS - 1	LCSW	13574	3.7016	-	7470A	PPB	17 Aug 2018 11:22:13	U	SMPL
PB112135TB - 1	PB112097TB	-177	-0.0432	-	7470A	PPB	17 Aug 2018 11:24:21	U	SMPL
J4269-02 - 1	AU-06-081518-A	-30	-0.0031	-	7470A	PPB	17 Aug 2018 11:26:29	U	SMPL
J4269-04 - 1	AU-06-081518-B	-25	-0.0018	-	7470A	PPB	17 Aug 2018 11:28:37	U	SMPL
J4282-06 - 1	SU-01-081518-A	1	0.0053	-	7470A	PPB	17 Aug 2018 11:30:45	U	SMPL
J4282-06DUP - 1	SU-01-081518-ADUP	-5	0.0037	-	7470A	PPB	17 Aug 2018 11:32:52	U	SMPL
CCV13 - 1	CCV13	18376	5.0094	-	7470A	PPB	17 Aug 2018 11:34:58	U	SMPL
CCB13 - 1	CCB13	-179	-0.0437	-	7470A	PPB	17 Aug 2018 11:37:05	U	SMPL
J4282-06MS - 1	SU-01-081518-AMS	13679	3.7302	-	7470A	PPB	17 Aug 2018 11:48:03	U	SMPL
J4282-06MSD - 1	SU-01-081518-AMSD	14185	3.8680	-	7470A	PPB	17 Aug 2018 11:50:09	U	SMPL
J4282-08 - 1	SU-01-081518-B	-147	-0.0350	-	7470A	PPB	17 Aug 2018 11:52:17	U	SMPL
J4486-03 - 1	VNJ202	49	0.0184	-	7470A	PPB	17 Aug 2018 11:54:25	U	SMPL
J4500-04 - 1	TP-1	-23	-0.0012	-	7470A	PPB	17 Aug 2018 11:56:32	U	SMPL
J4500-08 - 1	TP-2	-1	0.0048	-	7470A	PPB	17 Aug 2018 11:58:40	U	SMPL
J4500-12 - 1	TP-6	-1	0.0048	-	7470A	PPB	17 Aug 2018 12:00:48	U	SMPL
J4500-16 - 1	TP-7	16	0.0094	-	7470A	PPB	17 Aug 2018 12:02:56	U	SMPL
J4500-20 - 1	TP-12	3	0.0058	-	7470A	PPB	17 Aug 2018 12:05:04	U	SMPL
J4500-24 - 1	ROCK	26	0.0121	-	7470A	PPB	17 Aug 2018 12:07:11	U	SMPL
CCV14 - 1	CCV14	17948	4.8928	-	7470A	PPB	17 Aug 2018 12:09:18	U	SMPL
CCB14 - 1	CCB14	-138	-0.0325	-	7470A	PPB	17 Aug 2018 12:11:25	U	SMPL
J4502-02 - 1	LGS-DRUM	448	0.1270	-	7470A	PPB	17 Aug 2018 12:13:33	U	SMPL
PB112136BL - 1	PBW	-77	-0.0159	-	7470A	PPB	17 Aug 2018 12:15:40	U	SMPL
PB112136TB - 1	PB112099TB	51	0.0189	-	7470A	PPB	17 Aug 2018 12:19:53	U	SMPL
J4502-04 - 1	BROWN-FRAC-TANK	80	0.0268	-	7470A	PPB	17 Aug 2018 12:22:01	U	SMPL
J4502-04DUP - 1	BROWN-FRAC-TANKDUP	45	0.0173	-	7470A	PPB	17 Aug 2018 12:24:08	U	SMPL
J4502-04MS - 1	BROWN-FRAC-TANKMS	13840	3.7741	-	7470A	PPB	17 Aug 2018 12:28:21	U	SMPL
J4502-04MSD - 1	BROWN-FRAC-TANKMSD	13694	3.7343	-	7470A	PPB	17 Aug 2018 12:30:29	U	SMPL
PB112137BL - 1	PBW	-102	-0.0227	-	7470A	PPB	17 Aug 2018 12:32:39	U	SMPL
PB112137BS - 1	LCSW	13391	3.6518	-	7470A	PPB	17 Aug 2018 12:40:00	U	SMPL
PB112136BS - 1	LCSW	14584	3.9767	-	7470A	PPB	17 Aug 2018 12:42:06	U	SMPL
CCV15 - 1	CCV15	18603	5.0712	-	7470A	PPB	17 Aug 2018 12:44:15	U	SMPL
CCB15 - 1	CCB15	-153	-0.0366	-	7470A	PPB	17 Aug 2018 12:46:23	U	SMPL
J4489-01 - 1	SES-MS-PH4-COA-3QTR	-67	-0.0132	-	7470A	PPB	17 Aug 2018 12:48:31	U	SMPL
J4489-01DUP - 1	SES-MS-PH4-COA-3QTRDUP	-10	0.0023	-	7470A	PPB	17 Aug 2018 12:50:38	U	SMPL
J4489-01MS - 1	SES-MS-PH4-COA-3QTRMS	13186	3.5960	-	7470A	PPB	17 Aug 2018 12:52:45	U	SMPL
J4489-01MSD - 1	SES-MS-PH4-COA-3QTRMSD	14304	3.9004	-	7470A	PPB	17 Aug 2018 12:54:53	U	SMPL
J4282-06LX5 - 1		-102	-0.0227	-	7470A	PPB	17 Aug 2018 12:57:02	U	SMPL
J4282-06A - 1		14832	4.0442	-	7470A	PPB	17 Aug 2018 12:59:10	U	SMPL
J4502-04LX5 - 1		-91	-0.0197	-	7470A	PPB	17 Aug 2018 13:01:18	U	SMPL
J4502-04A - 1		13624	3.7153	-	7470A	PPB	17 Aug 2018 13:03:28	U	SMPL
J4489-01LX5 - 1		-97	-0.0214	-	7470A	PPB	17 Aug 2018 13:05:35	U	SMPL
J4489-01A - 1		14557	3.9693	-	7470A	PPB	17 Aug 2018 13:07:43	U	SMPL
CCV16 - 1	CCV16	18471	5.0352	-	7470A	PPB	17 Aug 2018 13:09:50	U	SMPL
CCB16 - 1	CCB16	-185	-0.0453	-	7470A	PPB	17 Aug 2018 13:11:57	U	SMPL