


LB97621

7470A

INSTRUMENT ID: CV1

Linear

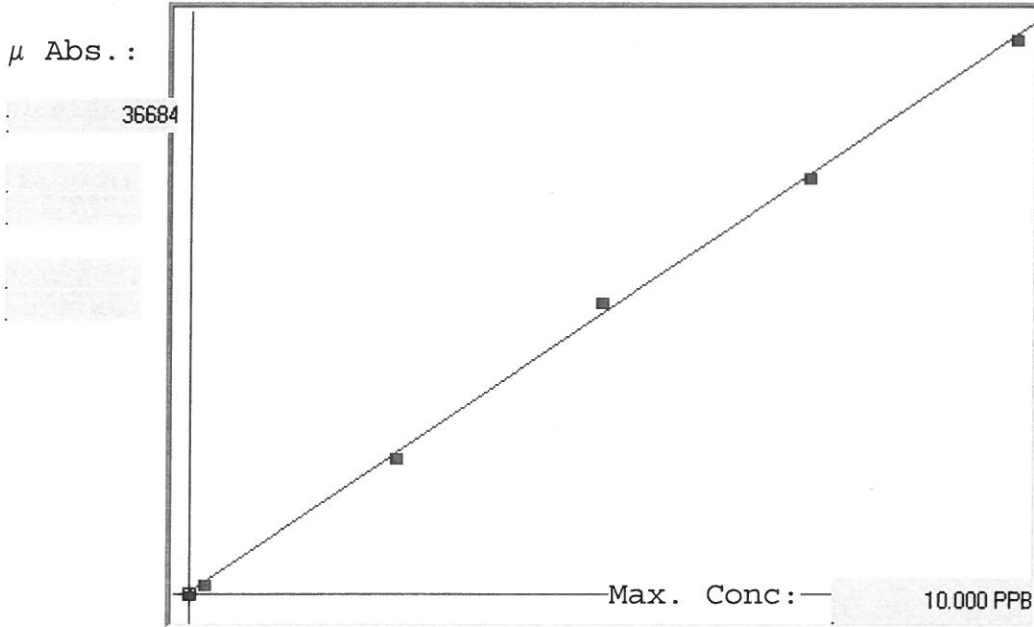

A= 0.0000e+000

B= 2.7136e-004

C= -2.5736e-002

Rho= 0.9996063

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.022	-0.022	14	0.000	14				
0.2	0.200	0.167	-0.033	711	0.0 %	711				
2.5	2.500	2.444	-0.056	9100	0.0 %	9100				
5.0	5.000	5.229	0.229	19364	0.0 %	19364				
7.5	7.500	7.454	-0.046	27563	0.0 %	27563				
10.0	10.000	9.929	-0.071	36684	0.0 %	36684				

LB97621 INSTRUMENT ID: CV1

Method: 7470A

Operator: Admin

Date of Analysis: 29 Aug 2018 15:05:23

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	14	-	0.0000	7470A	PPB	29 Aug 2018 15:07:16	S	Std
0.2 - 1	50.2	711	-	0.2000	7470A	PPB	29 Aug 2018 15:09:25	S	Std
2.5 - 1	52.5	9100	-	2.5000	7470A	PPB	29 Aug 2018 15:11:33	S	Std
5.0 - 1	55	19364	-	5.0000	7470A	PPB	29 Aug 2018 15:13:41	S	Std
7.5 - 1	57.5	27563	-	7.5000	7470A	PPB	29 Aug 2018 15:15:49	S	Std
10.0 - 1	510	36684	-	10.0000	7470A	PPB	29 Aug 2018 15:17:58	S	Std
ICV37 - 1	ICV37	13969	3.7648	-	7470A	PPB	29 Aug 2018 15:20:40	U	SMPL
ICB37 - 1	ICB37	-135	-0.0624	-	7470A	PPB	29 Aug 2018 15:22:46	U	SMPL
CCV28 - 1	CCV28	18042	4.8701	-	7470A	PPB	29 Aug 2018 15:24:53	U	SMPL
CCB28 - 1	CCB28	-155	-0.0678	-	7470A	PPB	29 Aug 2018 15:27:00	U	SMPL
CRA - 1	CRA	670	0.1561	-	7470A	PPB	29 Aug 2018 15:29:07	U	SMPL
HighStd - 1	HighStd	36148	9.7832	-	7470A	PPB	29 Aug 2018 15:31:14	U	SMPL
ChkStd - 1	ChkStd	25922	7.0084	-	7470A	PPB	29 Aug 2018 15:33:21	U	SMPL
PB112450BL - 1	PBW	-13	-0.0293	-	7470A	PPB	29 Aug 2018 15:37:57	U	SMPL
PB112450BS - 1	LCSW	14095	3.7990	-	7470A	PPB	29 Aug 2018 15:42:45	U	SMPL
PB112450TB - 1	PB112420TB	-114	-0.0567	-	7470A	PPB	29 Aug 2018 15:44:53	U	SMPL
J4274-06 - 1	HD-01-082718	2	-0.0252	-	7470A	PPB	29 Aug 2018 15:47:00	U	SMPL
J4274-06DUP - 1	HD-01-082718DUP	23	-0.0195	-	7470A	PPB	29 Aug 2018 15:49:09	U	SMPL
J4274-06MS - 1	HD-01-082718MS	12572	3.3858	-	7470A	PPB	29 Aug 2018 15:51:17	U	SMPL
J4274-06MSD - 1	HD-01-082718MSD	13141	3.5402	-	7470A	PPB	29 Aug 2018 15:53:24	U	SMPL
CCV29 - 1	CCV29	18265	4.9306	-	7470A	PPB	29 Aug 2018 15:55:30	U	SMPL
CCB29 - 1	CCB29	-131	-0.0613	-	7470A	PPB	29 Aug 2018 15:57:38	U	SMPL
J4276-06 - 1	OK-02-082718	15	-0.0217	-	7470A	PPB	29 Aug 2018 15:59:45	U	SMPL
J4277-10 - 1	OR-01-082718-A	25	-0.0190	-	7470A	PPB	29 Aug 2018 16:01:52	U	SMPL
J4277-12 - 1	OR-01-082718-B	35	-0.0162	-	7470A	PPB	29 Aug 2018 16:03:59	U	SMPL
J4661-03 - 1	WASTE-CLASS-HOT-SPOT	59	-0.0097	-	7470A	PPB	29 Aug 2018 16:06:06	U	SMPL
J4671-02 - 1	TL-SPEEDY-DRY	46	-0.0133	-	7470A	PPB	29 Aug 2018 16:08:13	U	SMPL
PB112453BL - 1	PBW	13	-0.0222	-	7470A	PPB	29 Aug 2018 16:10:21	U	SMPL
PB112453BS - 1	LCSW	12574	3.3863	-	7470A	PPB	29 Aug 2018 16:12:29	U	SMPL
J4658-01 - 1	PZ-1	-109	-0.0553	-	7470A	PPB	29 Aug 2018 16:14:37	U	SMPL
J4658-01DUP - 1	PZ-1DUP	-9	-0.0282	-	7470A	PPB	29 Aug 2018 16:16:45	U	SMPL
J4658-01MS - 1	PZ-1MS	12727	3.4278	-	7470A	PPB	29 Aug 2018 16:18:52	U	SMPL
CCV30 - 1	CCV30	18567	5.0125	-	7470A	PPB	29 Aug 2018 16:20:59	U	SMPL
CCB30 - 1	CCB30	-129	-0.0607	-	7470A	PPB	29 Aug 2018 16:23:06	U	SMPL
J4658-01MSD - 1	PZ-1MSD	13699	3.6916	-	7470A	PPB	29 Aug 2018 16:25:14	U	SMPL
J4658-02 - 1	PZ-2	-107	-0.0548	-	7470A	PPB	29 Aug 2018 16:27:21	U	SMPL
J4658-03 - 1	PZ-15	-1	-0.0260	-	7470A	PPB	29 Aug 2018 16:29:28	U	SMPL
J4658-04 - 1	GMW-10	-22	-0.0317	-	7470A	PPB	29 Aug 2018 16:31:35	U	SMPL
J4274-06LX5 - 1		39	-0.0152	-	7470A	PPB	29 Aug 2018 16:35:28	U	SMPL
J4274-06A - 1		15141	4.0829	-	7470A	PPB	29 Aug 2018 16:37:36	U	SMPL
J4658-01LX5 - 1		-104	-0.0540	-	7470A	PPB	29 Aug 2018 16:39:43	U	SMPL
J4658-01A - 1		14968	4.0359	-	7470A	PPB	29 Aug 2018 16:41:51	U	SMPL
CCV31 - 1	CCV31	18539	5.0049	-	7470A	PPB	29 Aug 2018 16:44:00	U	SMPL
CCB31 - 1	CCB31	-142	-0.0643	-	7470A	PPB	29 Aug 2018 16:46:07	U	SMPL