


7470A

LB97637
INSTRUMENT ID : CY1

Linear

 μ Abs.:

36223

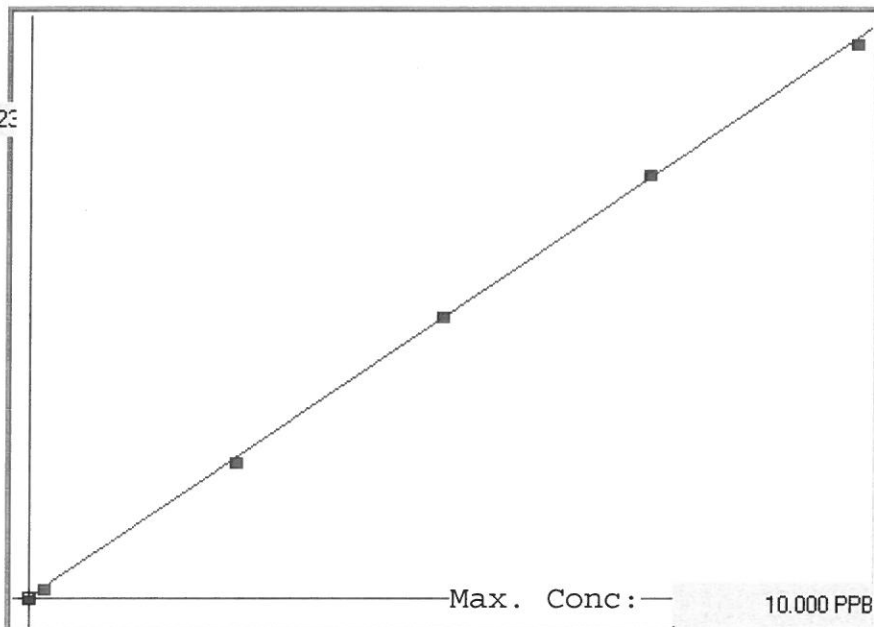

A= 0.0000e+000

B= 2.7379e-004

C= -8.2463e-003

Rho= 0.9998589

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.006	0.006	52	0.000	52				
0.2	0.200	0.172	-0.028	659	0.0 %	659				
2.5	2.500	2.458	-0.042	9008	0.0 %	9008				
5.0	5.000	5.066	0.066	18532	0.0 %	18532				
7.5	7.500	7.589	0.089	27749	0.0 %	27749				
10.0	10.000	9.909	-0.091	36223	0.0 %	36223				

LB97637 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 Aug 2018 14:38:05

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	52	-	0.0000	7470A	PPB	30 Aug 2018 14:40:00	S	Std
0.2 - 1	50.2	659	-	0.2000	7470A	PPB	30 Aug 2018 14:42:08	S	Std
2.5 - 1	52.5	9008	-	2.5000	7470A	PPB	30 Aug 2018 14:44:16	S	Std
5.0 - 1	55	18532	-	5.0000	7470A	PPB	30 Aug 2018 14:46:25	S	Std
7.5 - 1	57.5	27749	-	7.5000	7470A	PPB	30 Aug 2018 14:51:29	S	Std
10.0 - 1	510	36223	-	10.0000	7470A	PPB	30 Aug 2018 14:58:00	S	Std
ICV40 - 1	ICV40	14204	3.8806	-	7470A	PPB	30 Aug 2018 15:00:32	U	SMPL
ICB40 - 1	ICB40	-143	-0.0474	-	7470A	PPB	30 Aug 2018 15:02:38	U	SMPL
CCV41 - 1	CCV41	18669	5.1031	-	7470A	PPB	30 Aug 2018 15:04:46	U	SMPL
CCB41 - 1	CCB41	-143	-0.0474	-	7470A	PPB	30 Aug 2018 15:06:53	U	SMPL
CRA - 1	CRA	616	0.1604	-	7470A	PPB	30 Aug 2018 15:09:01	U	SMPL
HighStd - 1	HighStd	36502	9.9855	-	7470A	PPB	30 Aug 2018 15:11:08	U	SMPL
ChkStd - 1	ChkStd	25825	7.0623	-	7470A	PPB	30 Aug 2018 15:13:14	U	SMPL
PB112505BL - 1	PBW	-214	-0.0668	-	7470A	PPB	30 Aug 2018 15:15:24	U	SMPL
PB112505BS - 1	LCSW	13850	3.7837	-	7470A	PPB	30 Aug 2018 15:17:33	U	SMPL
PB112505TB - 1	PB112480TB	-112	-0.0389	-	7470A	PPB	30 Aug 2018 15:19:41	U	SMPL
J4275-20 - 1	CL-02-082918-A	-20	-0.0137	-	7470A	PPB	30 Aug 2018 15:21:49	U	SMPL
J4275-22 - 1	CL-02-082918-B	0	-0.0082	-	7470A	PPB	30 Aug 2018 15:23:57	U	SMPL
J4282-16 - 1	SU-01-082918-A	9	-0.0058	-	7470A	PPB	30 Aug 2018 15:26:06	U	SMPL
J4282-18 - 1	SU-01-082918-B	24	-0.0017	-	7470A	PPB	30 Aug 2018 15:28:13	U	SMPL
CCV42 - 1	CCV42	18458	5.0453	-	7470A	PPB	30 Aug 2018 15:30:19	U	SMPL
CCB42 - 1	CCB42	-144	-0.0477	-	7470A	PPB	30 Aug 2018 15:32:27	U	SMPL
J4282-20 - 1	SU-01-082918-C	0	-0.0082	-	7470A	PPB	30 Aug 2018 15:34:34	U	SMPL
J4699-03 - 1	CG-SOIL-1	21	-0.0025	-	7470A	PPB	30 Aug 2018 15:36:41	U	SMPL
J4699-03DUP - 1	CG-SOIL-1DUP	31	0.0002	-	7470A	PPB	30 Aug 2018 15:38:47	U	SMPL
J4699-03MS - 1	CG-SOIL-1MS	14184	3.8752	-	7470A	PPB	30 Aug 2018 15:40:54	U	SMPL
J4699-03MSD - 1	CG-SOIL-1MSD	13483	3.6832	-	7470A	PPB	30 Aug 2018 15:43:02	U	SMPL
J4699-06 - 1	CG-SOIL-2	-130	-0.0438	-	7470A	PPB	30 Aug 2018 15:45:10	U	SMPL
J4621-11 - 1	OILY-WATER	485	0.1245	-	7470A	PPB	30 Aug 2018 15:47:18	U	SMPL
J4699-03LX5 - 1		-41	-0.0195	-	7470A	PPB	30 Aug 2018 15:49:26	U	SMPL
J4699-03A - 1		14029	3.8327	-	7470A	PPB	30 Aug 2018 15:51:35	U	SMPL
CCV43 - 1	CCV43	18297	5.0012	-	7470A	PPB	30 Aug 2018 15:53:42	U	SMPL
CCB43 - 1	CCB43	-121	-0.0414	-	7470A	PPB	30 Aug 2018 15:55:49	U	SMPL