

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

9/4/2018 12:09

Test: Total CN mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.865	0.0	0.096	
ICB1	0.583	0.0	0.004	
CCV1	236.846	0.0	0.235	
CCB1	0.830	0.0	0.004	
PB112558BL	0.572	0.0	0.004	
PB112558BS	96.073	0.0	0.097	
MIDPB112558	235.273	0.0	0.233	
J4630-01	3.638	0.0	0.007	
J4630-01DUP	3.328	0.0	0.006	
J4630-01MS	35.804	0.0	0.038	
J4630-01MSD	35.158	0.0	0.037	
CCV2	252.214	0.0	0.250	
CCB2	0.850	0.0	0.004	

N	13
Mean	76.618
SD	99.8003
CV%	130.26

Aquakem v. 7.2AQ1

Results from time period:

Tue Sep 04 12:01:36 2018

Tue Sep 04 12:05:29 2018

AS

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.3636	µg/l	9/4/2018 10:16:42	
5.0PPBCN	A	Total CN	P	4.9527	µg/l	9/4/2018 10:16:43	
10PPBCN	A	Total CN	P	10.3965	µg/l	9/4/2018 10:16:44	
50PPBCN	A	Total CN	P	50.4276	µg/l	9/4/2018 10:16:45	
100PPBCN	A	Total CN	P	100.4026	µg/l	9/4/2018 10:16:46	
250PPBCN	A	Total CN	P	247.1754	µg/l	9/4/2018 10:16:47	
500PPBCN	A	Total CN	P	501.2816	µg/l	9/4/2018 10:16:48	
ICV1	S	Total CN	P	94.8655	µg/l	9/4/2018 12:01:36	
ICB1	S	Total CN	P	0.5826	µg/l	9/4/2018 12:01:37	
CCV1	S	Total CN	P	236.8463	µg/l	9/4/2018 12:01:38	
CCB1	S	Total CN	P	0.8295	µg/l	9/4/2018 12:01:39	
PB112558BL	S	Total CN	P	0.5721	µg/l	9/4/2018 12:01:40	
PB112558BS	S	Total CN	P	96.0729	µg/l	9/4/2018 12:01:41	
MIDPB112558	S	Total CN	P	235.2726	µg/l	9/4/2018 12:01:42	
J4630-01	S	Total CN	P	3.6382	µg/l	9/4/2018 12:01:43	
J4630-01DUP	S	Total CN	P	3.3279	µg/l	9/4/2018 12:01:44	
J4630-01MS	S	Total CN	P	35.8038	µg/l	9/4/2018 12:01:45	
J4630-01MSD	S	Total CN	P	35.1575	µg/l	9/4/2018 12:01:46	
CCV2	S	Total CN	P	252.2141	µg/l	9/4/2018 12:05:27	
CCB2	S	Total CN	P	0.8499	µg/l	9/4/2018 12:05:28	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

9/4/2018 10:25


Test Total CN

Accepted 9/4/2018 10:25

Factor 1021
Bias 0.003

Coeff. of det. 0.999950

Errors

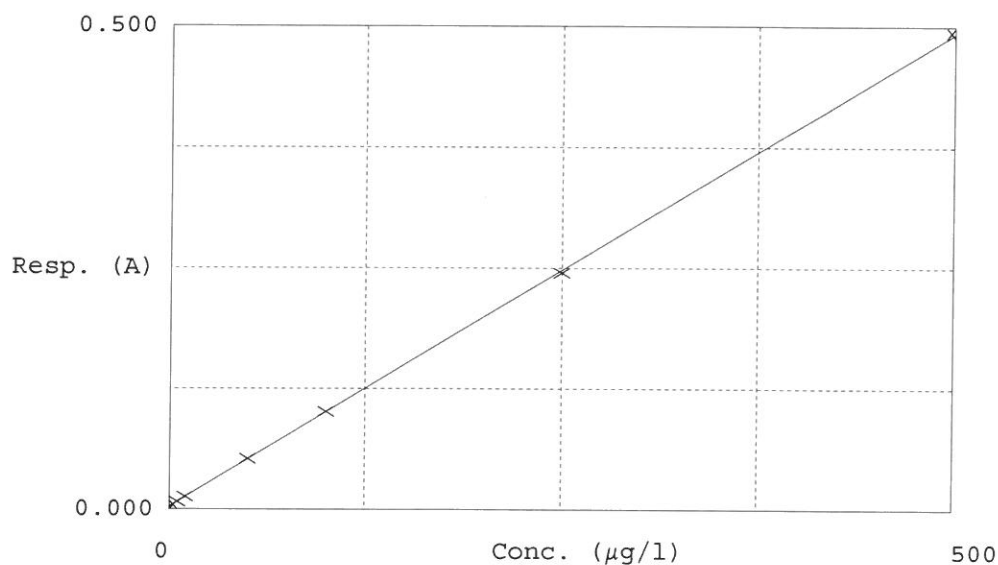

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.3636	0.0000	
2	5.0PPBCN	0.008	4.9527	5.0000	
3	10PPBCN	0.013	10.3965	10.0000	
4	50PPBCN	0.052	50.4276	50.0000	
5	100PPBCN	0.101	100.4026	100.0000	
6	250PPBCN	0.245	247.1754	250.0000	
7	500PPBCN	0.494	501.2816	500.0000	