


7470A

LB 97850
INSTRUMENT ID: CV1

Linear

 μ Abs.:

35803

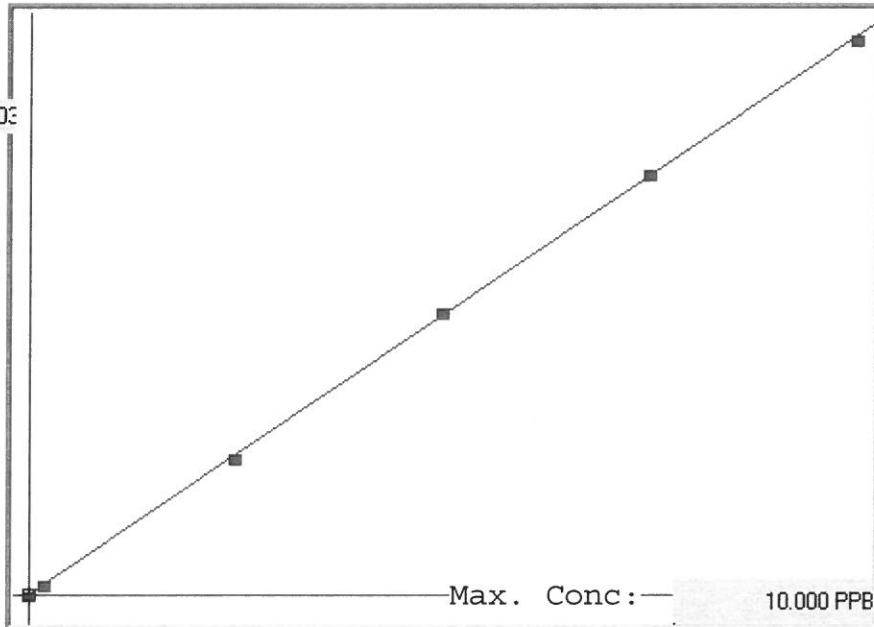

A= 0.0000e+000

B= 2.7733e-004

C= -1.1413e-003

Rho= 0.9998956

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.006	0.006	26	0.000	26				
0.2	0.200	0.172	-0.028	625	0.0 %	625				
2.5	2.500	2.459	-0.041	8871	0.0 %	8871				
5.0	5.000	5.080	0.080	18321	0.0 %	18321				
7.5	7.500	7.555	0.055	27246	0.0 %	27246				
10.0	10.000	9.928	-0.072	35803	0.0 %	35803				

LB97850 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Sep 2018 08:47:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	26	-	0.0000	7470A	PPB	12 Sep 2018 08:56:03	S	Std
0.2 - 1	50.2	625	-	0.2000	7470A	PPB	12 Sep 2018 08:58:11	S	Std
2.5 - 1	52.5	8871	-	2.5000	7470A	PPB	12 Sep 2018 09:00:21	S	Std
5.0 - 1	55	18321	-	5.0000	7470A	PPB	12 Sep 2018 09:02:29	S	Std
7.5 - 1	57.5	27246	-	7.5000	7470A	PPB	12 Sep 2018 09:04:39	S	Std
10.0 - 1	59	35803	-	10.0000	7470A	PPB	12 Sep 2018 09:06:47	S	Std
ICV59 - 1	ICV59	14478	4.0140	-	7470A	PPB	12 Sep 2018 09:09:24	U	SMPL
ICB59 - 1	ICB59	-223	-0.0630	-	7470A	PPB	12 Sep 2018 09:11:33	U	SMPL
CCV34 - 1	CCV34	18133	5.0276	-	7470A	PPB	12 Sep 2018 09:13:42	U	SMPL
CCB34 - 1	CCB34	-252	-0.0710	-	7470A	PPB	12 Sep 2018 09:15:49	U	SMPL
CRA - 1	CRA	713	0.1966	-	7470A	PPB	12 Sep 2018 09:17:58	U	SMPL
HighStd - 1	HighStd	35674	9.8922	-	7470A	PPB	12 Sep 2018 09:20:05	U	SMPL
ChkStd - 1	ChkStd	25996	7.2083	-	7470A	PPB	12 Sep 2018 09:22:11	U	SMPL
PB112769BL - 1	PBW	-300	-0.0843	-	7470A	PPB	12 Sep 2018 09:24:21	U	SMPL
PB112769BS - 1	LCSW	13225	3.6665	-	7470A	PPB	12 Sep 2018 09:26:30	U	SMPL
PB112769TB - 1	PB112747TB	-283	-0.0796	-	7470A	PPB	12 Sep 2018 09:28:38	U	SMPL
J4724-19 - 1	EP1-SUT-4USTS-SB	-178	-0.0505	-	7470A	PPB	12 Sep 2018 09:30:48	U	SMPL
J4838-09 - 1	SUP-1A-C-090718-1	6	0.0005	-	7470A	PPB	12 Sep 2018 09:32:57	U	SMPL
J4838-10 - 1	SUP-1B-C-090718-1	4	-0.0000	-	7470A	PPB	12 Sep 2018 09:35:05	U	SMPL
J4840-01 - 1	OILY-DEBRIS	83	0.0219	-	7470A	PPB	12 Sep 2018 09:37:12	U	SMPL
CCV35 - 1	CCV35	18359	5.0903	-	7470A	PPB	12 Sep 2018 09:39:19	U	SMPL
CCB35 - 1	CCB35	-162	-0.0461	-	7470A	PPB	12 Sep 2018 09:41:26	U	SMPL
J4842-18 - 1	SG-SOIL	-205	-0.0580	-	7470A	PPB	12 Sep 2018 09:43:33	U	SMPL
J4842-18DUP - 1	SG-SOILDUP	-53	-0.0158	-	7470A	PPB	12 Sep 2018 09:45:40	U	SMPL
J4842-18MS - 1	SG-SOILMS	12849	3.5622	-	7470A	PPB	12 Sep 2018 09:47:47	U	SMPL
J4842-18MSD - 1	SG-SOILMSD	13105	3.6332	-	7470A	PPB	12 Sep 2018 09:49:54	U	SMPL
J4842-18LX5 - 1		-79	-0.0231	-	7470A	PPB	12 Sep 2018 09:52:03	U	SMPL
J4842-18A - 1		12315	3.4141	-	7470A	PPB	12 Sep 2018 09:54:12	U	SMPL
CCV36 - 1	CCV36	18216	5.0507	-	7470A	PPB	12 Sep 2018 09:56:20	U	SMPL
CCB36 - 1	CCB36	-218	-0.0616	-	7470A	PPB	12 Sep 2018 09:58:29	U	SMPL