


7470A

LB97880
INSTRUMENT ID: LV1

Linear

 μ Abs.:

37591

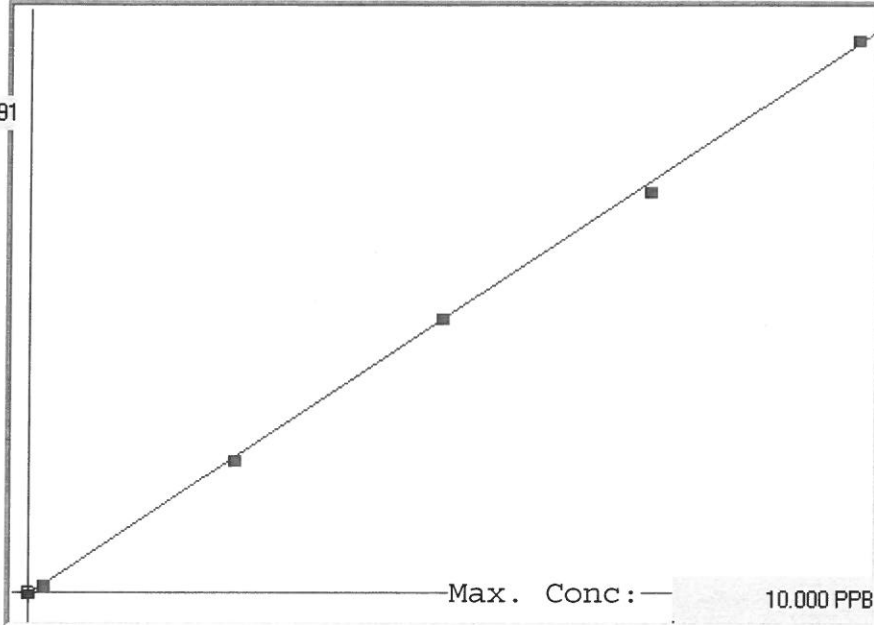

A= 0.0000e+000

B= 2.6720e-004

C= 5.0815e-002

Rho= 0.9997717

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.026	0.026	-94	0.000	-94				
0.2	0.200	0.214	0.014	609	0.0 %	609				
2.5	2.500	2.472	-0.028	9061	0.0 %	9061				
5.0	5.000	5.050	0.050	18708	0.0 %	18708				
7.5	7.500	7.344	-0.156	27297	0.0 %	27297				
10.0	10.000	10.095	0.095	37591	0.0 %	37591				

LB97880 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Sep 2018 10:33:01

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-94	-	0.00007470A	PPB		13 Sep 2018 10:37:26	S	Std
0.2 - 1	50.2	609	-	0.20007470A	PPB		13 Sep 2018 10:39:34	S	Std
2.5 - 1	52.5	9061	-	2.50007470A	PPB		13 Sep 2018 10:41:44	S	Std
5.0 - 1	55	18708	-	5.00007470A	PPB		13 Sep 2018 10:43:53	S	Std
7.5 - 1	57.5	27297	-	7.50007470A	PPB		13 Sep 2018 10:46:02	S	Std
10.0 - 1	510	37591	-	10.00007470A	PPB		13 Sep 2018 10:50:39	S	Std
ICV62 - 1	ICV62	13413	3.6347	-7470A	PPB		13 Sep 2018 10:53:12	U	SMPL
ICB62 - 1	ICB62	-164	0.0070	-7470A	PPB		13 Sep 2018 10:55:20	U	SMPL
CCV44 - 1	CCV44	19233	5.1898	-7470A	PPB		13 Sep 2018 10:57:27	U	SMPL
CCB44 - 1	CCB44	-217	-0.0072	-7470A	PPB		13 Sep 2018 10:59:34	U	SMPL
CRA - 1	CRA	641	0.2221	-7470A	PPB		13 Sep 2018 11:01:43	U	SMPL
HighStd - 1	HighStd	37742	10.1353	-7470A	PPB		13 Sep 2018 11:03:49	U	SMPL
ChkStd - 1	ChkStd	25483	6.8597	-7470A	PPB		13 Sep 2018 11:05:57	U	SMPL
PB112792BL - 1	PBW	-316	-0.0336	-7470A	PPB		13 Sep 2018 11:08:06	U	SMPL
PB112792BS - 1	LCSW	13851	3.7517	-7470A	PPB		13 Sep 2018 11:10:16	U	SMPL
PB112792TB - 1	PB112766TB	-235	-0.0120	-7470A	PPB		13 Sep 2018 11:12:24	U	SMPL
J4780-02 - 1	TR-04-091118	-15	0.0468	-7470A	PPB		13 Sep 2018 11:14:32	U	SMPL
J4780-02DUP - 1	TR-04-091118DUP	-8	0.0487	-7470A	PPB		13 Sep 2018 11:16:40	U	SMPL
J4780-02MS - 1	TR-04-091118MS	13515	3.6620	-7470A	PPB		13 Sep 2018 11:18:49	U	SMPL
J4780-02MSD - 1	TR-04-091118MSD	14195	3.8437	-7470A	PPB		13 Sep 2018 11:20:55	U	SMPL
CCV45 - 1	CCV45	19233	5.1898	-7470A	PPB		13 Sep 2018 11:23:02	U	SMPL
CCB45 - 1	CCB45	-346	-0.0416	-7470A	PPB		13 Sep 2018 11:25:09	U	SMPL
J4853-04 - 1	CS-SOIL	8	0.0530	-7470A	PPB		13 Sep 2018 11:27:17	U	SMPL
J4856-04 - 1	STONE-PILE	-71	0.0318	-7470A	PPB		13 Sep 2018 11:29:24	U	SMPL
J4856-11 - 1	TP-1-3	-48	0.0380	-7470A	PPB		13 Sep 2018 11:31:31	U	SMPL
J4780-02LX5 - 1		-2	0.0503	-7470A	PPB		13 Sep 2018 11:33:38	U	SMPL
J4780-02A - 1		15100	4.0855	-7470A	PPB		13 Sep 2018 11:38:20	U	SMPL
CCV46 - 1	CCV46	19134	5.1633	-7470A	PPB		13 Sep 2018 11:40:28	U	SMPL
CCB46 - 1	CCB46	-204	-0.0037	-7470A	PPB		13 Sep 2018 11:42:37	U	SMPL