


7470A

LB 98078
INSTRUMENT ID: CV1

Linear

 μ Abs.:

35620

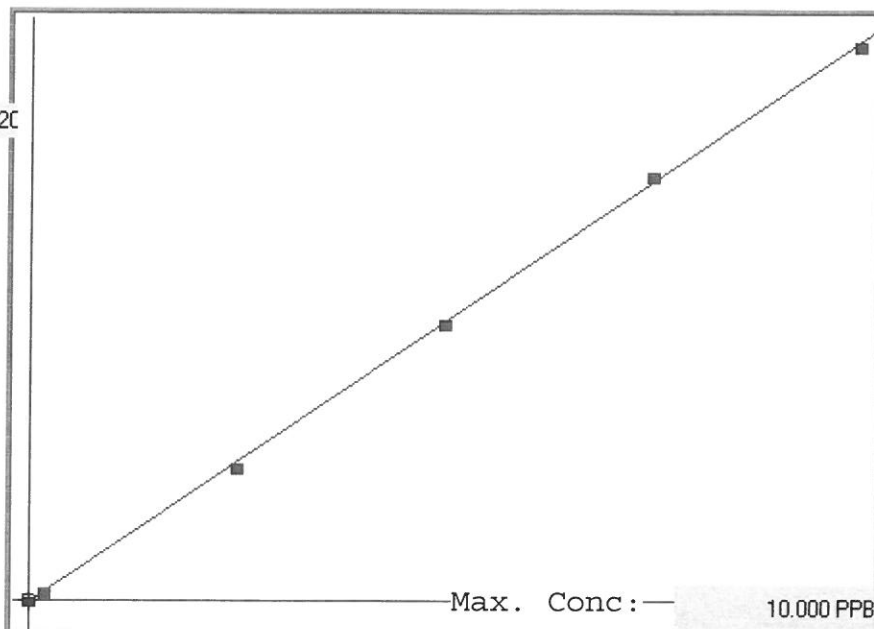

A= 0.0000e+000

B= 2.7788e-004

C= 3.3004e-002

Rho= 0.9998370

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.044	0.044	41	0.000	41				
0.2	0.200	0.188	-0.012	559	0.0 %	559				
2.5	2.500	2.425	-0.075	8609	0.0 %	8609				
5.0	5.000	4.992	-0.008	17846	0.0 %	17846				
7.5	7.500	7.619	0.119	27299	0.0 %	27299				
10.0	10.000	9.931	-0.069	35620	0.0 %	35620				

LB98078 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Sep 2018 09:14:18

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	41	-	0.0000	7470A	PPB	21 Sep 2018 09:20:10	S	Std
0.2 - 1	50.2	559	-	0.2000	7470A	PPB	21 Sep 2018 09:22:19	S	Std
2.5 - 1	52.5	8609	-	2.5000	7470A	PPB	21 Sep 2018 09:24:27	S	Std
5.0 - 1	55	17846	-	5.0000	7470A	PPB	21 Sep 2018 09:26:35	S	Std
7.5 - 1	57.5	27299	-	7.5000	7470A	PPB	21 Sep 2018 09:28:44	S	Std
10.0 - 1	510	35620	-	10.0000	7470A	PPB	21 Sep 2018 09:30:52	S	Std
ICV76 - 1	ICV76	14069	3.9425	-	7470A	PPB	21 Sep 2018 09:33:28	U	SMPL
ICB76 - 1	ICB76	-30	0.0247	-	7470A	PPB	21 Sep 2018 09:35:36	U	SMPL
CCV40 - 1	CCV40	18349	5.1318	-	7470A	PPB	21 Sep 2018 09:37:43	U	SMPL
CCB40 - 1	CCB40	-23	0.0266	-	7470A	PPB	21 Sep 2018 09:39:50	U	SMPL
CRA - 1	CRA	597	0.1989	-	7470A	PPB	21 Sep 2018 09:41:58	U	SMPL
HighStd - 1	HighStd	36174	10.0850	-	7470A	PPB	21 Sep 2018 09:44:05	U	SMPL
ChkStd - 1	ChkStd	24723	6.9030	-	7470A	PPB	21 Sep 2018 09:46:11	U	SMPL
PB113080BL - 1	PBW	-450	-0.0920	-	7470A	PPB	21 Sep 2018 09:48:20	U	SMPL
PB113080BS - 1	LCSW	12468	3.4976	-	7470A	PPB	21 Sep 2018 09:50:30	U	SMPL
PB113080TB - 1	PB113044TB	-143	-0.0067	-	7470A	PPB	21 Sep 2018 09:52:38	U	SMPL
J4778-02 - 1	SA-01-091918	-1	0.0327	-	7470A	PPB	21 Sep 2018 09:54:46	U	SMPL
J4985-02 - 1	EDISON-1	49	0.0466	-	7470A	PPB	21 Sep 2018 09:56:54	U	SMPL
J4985-04 - 1	EDISON-2	-66	0.0147	-	7470A	PPB	21 Sep 2018 09:59:03	U	SMPL
J4987-03 - 1	RBR200036	-64	0.0152	-	7470A	PPB	21 Sep 2018 10:01:12	U	SMPL
CCV41 - 1	CCV41	18084	5.0582	-	7470A	PPB	21 Sep 2018 10:03:19	U	SMPL
CCB41 - 1	CCB41	-137	-0.0051	-	7470A	PPB	21 Sep 2018 10:05:28	U	SMPL
J4988-02 - 1	METUCHEN-1.5	-52	0.0186	-	7470A	PPB	21 Sep 2018 10:07:35	U	SMPL
J4988-04 - 1	METUCHEN-2	-54	0.0180	-	7470A	PPB	21 Sep 2018 10:09:41	U	SMPL
J4988-06 - 1	METUCHEN-3	-36	0.0230	-	7470A	PPB	21 Sep 2018 10:11:49	U	SMPL
J4988-08 - 1	METUCHEN-4	65	0.0511	-	7470A	PPB	21 Sep 2018 10:13:56	U	SMPL
J4993-05 - 1	NS-SLUDGE	91	0.0583	-	7470A	PPB	21 Sep 2018 10:16:03	U	SMPL
J5001-01 - 1	BS-OILY-DEBRI	-57	0.0172	-	7470A	PPB	21 Sep 2018 10:18:11	U	SMPL
J5001-04 - 1	BS-OILY-STONE	-35	0.0233	-	7470A	PPB	21 Sep 2018 10:25:17	U	SMPL
J5001-04DUP - 1	BS-OILY-STONEDUP	-125	-0.0017	-	7470A	PPB	21 Sep 2018 10:27:25	U	SMPL
J5001-04MS - 1	BS-OILY-STONEMS	13889	3.8925	-	7470A	PPB	21 Sep 2018 10:29:35	U	SMPL
J5001-04MSD - 1	BS-OILY-STONEMSD	14055	3.9386	-	7470A	PPB	21 Sep 2018 10:34:19	U	SMPL
CCV42 - 1	CCV42	18131	5.0712	-	7470A	PPB	21 Sep 2018 10:36:26	U	SMPL
CCB42 - 1	CCB42	-76	0.0119	-	7470A	PPB	21 Sep 2018 10:38:33	U	SMPL
PB113082BL - 1	PBW	-173	-0.0151	-	7470A	PPB	21 Sep 2018 10:40:42	U	SMPL
PB113082BS - 1	LCSW	13473	3.7769	-	7470A	PPB	21 Sep 2018 10:42:49	U	SMPL
PB113082TB - 1	PB113047TB	-209	-0.0251	-	7470A	PPB	21 Sep 2018 10:44:55	U	SMPL
J4993-07 - 1	NS-OILY-WATER	-41	0.0216	-	7470A	PPB	21 Sep 2018 10:47:05	U	SMPL
J4993-07DUP - 1	NS-OILY-WATERDUP	-24	0.0263	-	7470A	PPB	21 Sep 2018 10:49:12	U	SMPL
J4993-07MS - 1	NS-OILY-WATERMS	12543	3.5185	-	7470A	PPB	21 Sep 2018 10:51:20	U	SMPL
J4993-07MSD - 1	NS-OILY-WATERMSD	12762	3.5793	-	7470A	PPB	21 Sep 2018 10:53:28	U	SMPL
PB113083BL - 1	PBW	-173	-0.0151	-	7470A	PPB	21 Sep 2018 10:55:36	U	SMPL
PB113083BS - 1	LCSW	13993	3.9214	-	7470A	PPB	21 Sep 2018 10:57:45	U	SMPL
J4993-06 - 1	NS-OILY-WATER	573	0.1922	-	7470A	PPB	21 Sep 2018 10:59:52	U	SMPL
CCV43 - 1	CCV43	17864	4.9971	-	7470A	PPB	21 Sep 2018 11:02:02	U	SMPL
CCB43 - 1	CCB43	-71	0.0133	-	7470A	PPB	21 Sep 2018 11:04:09	U	SMPL
J4993-06DUP - 1	NS-OILY-WATERDUP	413	0.1478	-	7470A	PPB	21 Sep 2018 11:06:18	U	SMPL
J4993-06MS - 1	NS-OILY-WATERMS	12993	3.6435	-	7470A	PPB	21 Sep 2018 11:08:26	U	SMPL
J4993-06MSD - 1	NS-OILY-WATERMSD	13038	3.6560	-	7470A	PPB	21 Sep 2018 11:10:33	U	SMPL
J5001-04LX5 - 1		-216	-0.0270	-	7470A	PPB	21 Sep 2018 11:12:41	U	SMPL
J5001-04A - 1		14231	3.9875	-	7470A	PPB	21 Sep 2018 11:14:51	U	SMPL
J4993-07LX5 - 1		-164	-0.0126	-	7470A	PPB	21 Sep 2018 11:16:59	U	SMPL
J4993-07A - 1		13915	3.8997	-	7470A	PPB	21 Sep 2018 11:19:07	U	SMPL
J4993-06LX5 - 1		-34	0.0236	-	7470A	PPB	21 Sep 2018 11:21:16	U	SMPL
J4993-06A - 1		15305	4.2860	-	7470A	PPB	21 Sep 2018 11:23:25	U	SMPL
CCV44 - 1	CCV44	18398	5.1454	-	7470A	PPB	21 Sep 2018 11:25:32	U	SMPL
CCB44 - 1	CCB44	-52	0.0186	-	7470A	PPB	21 Sep 2018 11:27:42	U	SMPL