


LB98112

7470A

INSTRUMENT ID : CV4

 μ Abs.:

35303

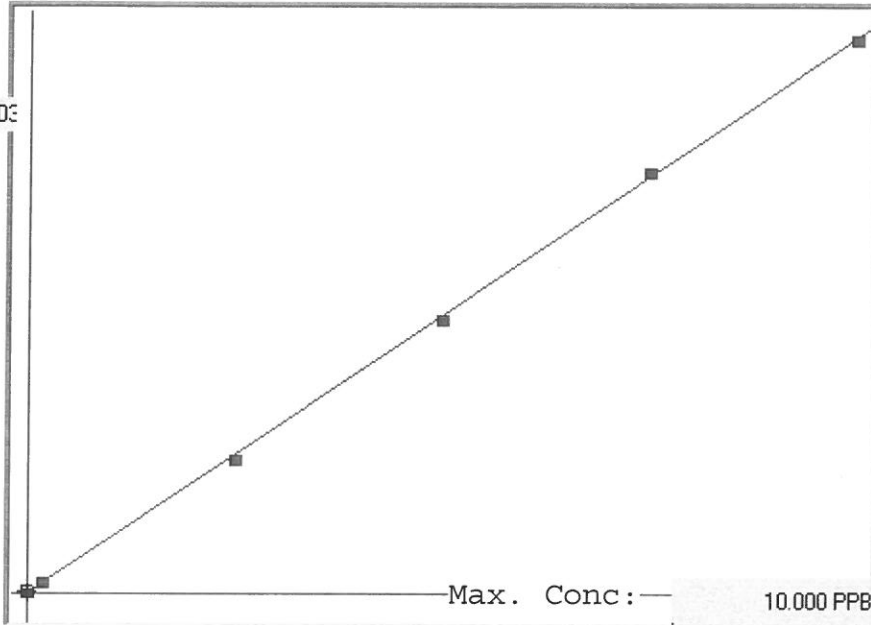

Linear

A= 0.0000e+000

B= 2.8260e-004

C= -3.5907e-003

Rho= 0.9998788

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.046	0.046	175	0.000	175				
0.2	0.200	0.215	0.015	773	0.0 %	773				
2.5	2.500	2.427	-0.073	8599	0.0 %	8599				
5.0	5.000	4.947	-0.053	17518	0.0 %	17518				
7.5	7.500	7.593	0.093	26879	0.0 %	26879				
10.0	10.000	9.973	-0.027	35303	0.0 %	35303				

LB98112 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 24 Sep 2018 13:08:46

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	175	-	0.0000	7470A	PPB	24 Sep 2018 13:47:31	S	Std
0.2 - 1	50.2	773	-	0.2000	7470A	PPB	24 Sep 2018 13:49:40	S	Std
2.5 - 1	52.5	8599	-	2.5000	7470A	PPB	24 Sep 2018 13:51:48	S	Std
5.0 - 1	55	17518	-	5.0000	7470A	PPB	24 Sep 2018 13:53:57	S	Std
7.5 - 1	57.5	26879	-	7.5000	7470A	PPB	24 Sep 2018 13:56:05	S	Std
10.0 - 1	59	35303	-	10.0000	7470A	PPB	24 Sep 2018 14:00:51	S	Std
ICV79 - 1	ICV79	13657	3.8559	-	7470A	PPB	24 Sep 2018 14:03:25	U	SMPL
ICB79 - 1	ICB79	-81	-0.0265	-	7470A	PPB	24 Sep 2018 14:05:32	U	SMPL
CCV59 - 1	CCV59	17480	4.9363	-	7470A	PPB	24 Sep 2018 14:07:41	U	SMPL
CCB59 - 1	CCB59	-71	-0.0237	-	7470A	PPB	24 Sep 2018 14:09:47	U	SMPL
CRA - 1	CRA	745	0.2069	-	7470A	PPB	24 Sep 2018 14:11:55	U	SMPL
HighStd - 1	HighStd	35852	10.1283	-	7470A	PPB	24 Sep 2018 14:14:02	U	SMPL
ChkStd - 1	ChkStd	25264	7.1361	-	7470A	PPB	24 Sep 2018 14:16:09	U	SMPL
PB113118BL - 1	PBW	-335	-0.0983	-	7470A	PPB	24 Sep 2018 14:18:19	U	SMPL
PB113118BS - 1	LCSW	14535	4.1041	-	7470A	PPB	24 Sep 2018 14:20:29	U	SMPL
PB113118TB - 1	PB113085TB	-148	-0.0454	-	7470A	PPB	24 Sep 2018 14:22:36	U	SMPL
J4777-12 - 1	PL-02-0920-18-A	-4	-0.0047	-	7470A	PPB	24 Sep 2018 14:24:44	U	SMPL
J4777-14 - 1	PL-02-0920-18-B	36	0.0066	-	7470A	PPB	24 Sep 2018 14:26:53	U	SMPL
J4777-16 - 1	PL-02-0920-18-C	29	0.0046	-	7470A	PPB	24 Sep 2018 14:29:01	U	SMPL
J4777-18 - 1	PL-02-0920-18-D	5	-0.0022	-	7470A	PPB	24 Sep 2018 14:31:08	U	SMPL
CCV60 - 1	CCV60	17628	4.9781	-	7470A	PPB	24 Sep 2018 14:33:15	U	SMPL
CCB60 - 1	CCB60	-84	-0.0273	-	7470A	PPB	24 Sep 2018 14:35:22	U	SMPL
J4777-20 - 1	PL-03-092018-A	18	0.0015	-	7470A	PPB	24 Sep 2018 14:37:29	U	SMPL
J4777-22 - 1	PL-03-092018-B	12	-0.0002	-	7470A	PPB	24 Sep 2018 14:39:36	U	SMPL
J4777-24 - 1	PL-03-092018-C	36	0.0066	-	7470A	PPB	24 Sep 2018 14:41:43	U	SMPL
J4777-26 - 1	PL-04-092018-A	50	0.0105	-	7470A	PPB	24 Sep 2018 14:43:50	U	SMPL
J4777-28 - 1	PL-04-092018-B	1	-0.0033	-	7470A	PPB	24 Sep 2018 14:45:57	U	SMPL
J4777-30 - 1	PL-04-092018-C	34	0.0060	-	7470A	PPB	24 Sep 2018 14:48:05	U	SMPL
J4777-32 - 1	PL-04-092018-D	21	0.0023	-	7470A	PPB	24 Sep 2018 14:50:13	U	SMPL
J5021-04 - 1	LS-SOIL-A	58	0.0128	-	7470A	PPB	24 Sep 2018 14:52:22	U	SMPL
J5021-08 - 1	LS-SOIL-B	-1	-0.0039	-	7470A	PPB	24 Sep 2018 14:54:30	U	SMPL
J5021-12 - 1	LS-SOIL-C	43	0.0086	-	7470A	PPB	24 Sep 2018 14:56:37	U	SMPL
CCV61 - 1	CCV61	17251	4.8716	-	7470A	PPB	24 Sep 2018 14:58:44	U	SMPL
CCB61 - 1	CCB61	-90	-0.0290	-	7470A	PPB	24 Sep 2018 15:00:51	U	SMPL
J5021-16 - 1	LS-SOIL-D	-37	-0.0140	-	7470A	PPB	24 Sep 2018 15:02:59	U	SMPL
J5021-20 - 1	LS-SOIL-E	-6	-0.0053	-	7470A	PPB	24 Sep 2018 15:05:06	U	SMPL
J5023-04 - 1	NB-PIT-1	30	0.0049	-	7470A	PPB	24 Sep 2018 15:07:13	U	SMPL
J5023-08 - 1	NB-PIT-2	185	0.0487	-	7470A	PPB	24 Sep 2018 15:09:20	U	SMPL
J5023-12 - 1	NB-PIT-3	61	0.0136	-	7470A	PPB	24 Sep 2018 15:11:27	U	SMPL
J5023-12DUP - 1	NB-PIT-3DUP	39	0.0074	-	7470A	PPB	24 Sep 2018 15:13:35	U	SMPL
J5023-12MS - 1	NB-PIT-3MS	12810	3.6166	-	7470A	PPB	24 Sep 2018 15:15:44	U	SMPL
J5023-12MSD - 1	NB-PIT-3MSD	12556	3.5448	-	7470A	PPB	24 Sep 2018 15:17:52	U	SMPL
J5023-12LX5 - 1		0	-0.0036	-	7470A	PPB	24 Sep 2018 15:20:01	U	SMPL
J5023-12A - 1		14137	3.9916	-	7470A	PPB	24 Sep 2018 15:22:08	U	SMPL
CCV62 - 1	CCV62	17607	4.9722	-	7470A	PPB	24 Sep 2018 15:24:15	U	SMPL
CCB62 - 1	CCB62	-53	-0.0186	-	7470A	PPB	24 Sep 2018 15:26:22	U	SMPL