

L398147


7470A

INSTRUMENT ID: CV2

Linear

μ Abs.:

29894

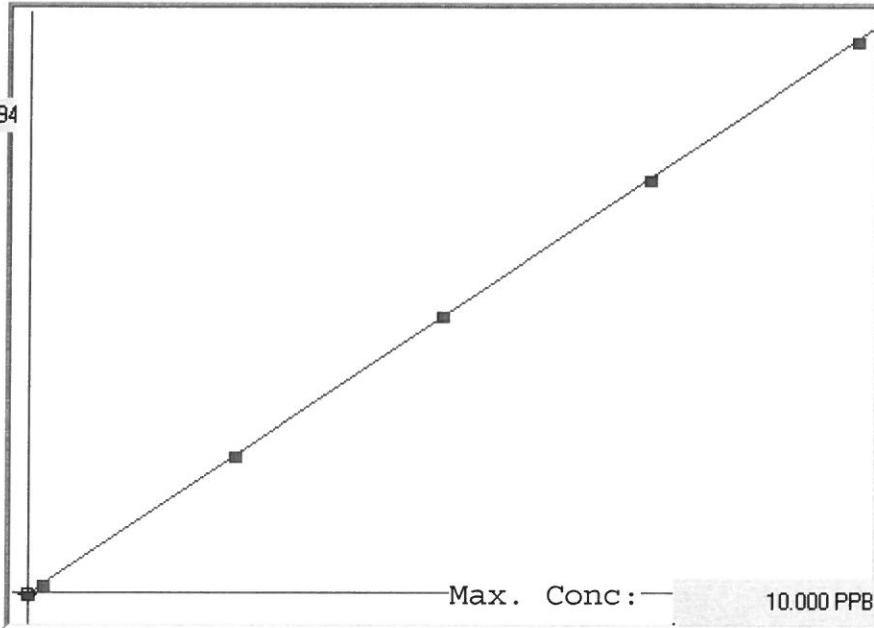

A= 0.0000e+000

B= 3.3315e-004

C= 3.4903e-002

Rho= 0.9999349

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.001	-0.001	-109	0.000	-109				
0.2	0.200	0.196	-0.004	485	0.0 %	485				
2.5	2.500	2.492	-0.008	7374	0.0 %	7374				
5.0	5.000	5.026	0.026	14981	0.0 %	14981				
7.5	7.500	7.493	-0.007	22387	0.0 %	22387				
10.0	10.000	9.994	-0.006	29894	0.0 %	29894				

LB98147 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 26 Sep 2018 07:44:09

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-109	-	0.0007470A	PPB		26 Sep 2018 07:47:33	S	Std
0.2 - 1	50.2	485	-	0.20007470A	PPB		26 Sep 2018 07:49:41	S	Std
2.5 - 1	52.5	7374	-	2.50007470A	PPB		26 Sep 2018 07:51:52	S	Std
5.0 - 1	55	14981	-	5.00007470A	PPB		26 Sep 2018 07:54:04	S	Std
7.5 - 1	57.5	22387	-	7.50007470A	PPB		26 Sep 2018 07:56:13	S	Std
10.0 - 1	59	29894	-	10.00007470A	PPB		26 Sep 2018 07:58:24	S	Std
ICV82 - 1	ICV82	11504	3.8675	-7470A	PPB		26 Sep 2018 08:01:01	U	SMPL
ICB82 - 1	ICB82	-280	-0.0584	-7470A	PPB		26 Sep 2018 08:03:09	U	SMPL
CCV81 - 1	CCV81	14729	4.9419	-7470A	PPB		26 Sep 2018 08:05:16	U	SMPL
CCB81 - 1	CCB81	-208	-0.0344	-7470A	PPB		26 Sep 2018 08:07:25	U	SMPL
CRA - 1	CRA	490	0.1981	-7470A	PPB		26 Sep 2018 08:09:34	U	SMPL
HighStd - 1	HighStd	32571	10.8861	-7470A	PPB		26 Sep 2018 08:11:42	U	SMPL
ChkStd - 1	ChkStd	21918	7.3370	-7470A	PPB		26 Sep 2018 08:13:49	U	SMPL
PB113168BL - 1	PBW	-198	-0.0311	-7470A	PPB		26 Sep 2018 08:15:57	U	SMPL
PB113168BS - 1	LCSW	11148	3.7489	-7470A	PPB		26 Sep 2018 08:18:08	U	SMPL
PB113168TB - 1	PB113124TB	-207	-0.0341	-7470A	PPB		26 Sep 2018 08:20:16	U	SMPL
J4770-02 - 1	JC-02-092118-A	-18	0.0289	-7470A	PPB		26 Sep 2018 08:22:25	U	SMPL
J4770-04 - 1	JC-02-092118-B	-45	0.0199	-7470A	PPB		26 Sep 2018 08:24:33	U	SMPL
J4770-06 - 1	JC-02-092118-C	142	0.0822	-7470A	PPB		26 Sep 2018 08:26:42	U	SMPL
J4770-08 - 1	JC-02-092118-D	136	0.0802	-7470A	PPB		26 Sep 2018 08:28:48	U	SMPL
CCV82 - 1	CCV82	15202	5.0995	-7470A	PPB		26 Sep 2018 08:30:55	U	SMPL
CCB82 - 1	CCB82	-116	-0.0037	-7470A	PPB		26 Sep 2018 08:33:02	U	SMPL
J4770-10 - 1	JC-02-092118-E	5	0.0366	-7470A	PPB		26 Sep 2018 08:35:10	U	SMPL
J4770-12 - 1	JC-02-092118-F	14	0.0396	-7470A	PPB		26 Sep 2018 08:37:16	U	SMPL
J4770-14 - 1	JC-02-092118-G	-37	0.0226	-7470A	PPB		26 Sep 2018 08:39:24	U	SMPL
J4770-16 - 1	JC-02-092118-H	82	0.0622	-7470A	PPB		26 Sep 2018 08:41:31	U	SMPL
J4770-18 - 1	JC-02-092118-I	1	0.0352	-7470A	PPB		26 Sep 2018 08:43:38	U	SMPL
J4770-20 - 1	JC-02-092118-J	66	0.0569	-7470A	PPB		26 Sep 2018 08:45:47	U	SMPL
J5042-05 - 1	2018-NYSEG-CLARK-PH4-AREA-12-BANK	-23	0.0272	-7470A	PPB		26 Sep 2018 08:47:55	U	SMPL
J5042-06 - 1	2018-NYSEG-CLARK-PH4-AREA-14-BANK1	33	0.0459	-7470A	PPB		26 Sep 2018 08:50:04	U	SMPL
J5042-07 - 1	2018-NYSEG-CLARK-PH4-AREA-14-BANK2	79	0.0612	-7470A	PPB		26 Sep 2018 08:52:15	U	SMPL
J5042-08 - 1	2018-NYSEG-CLARK-PH4-AREA-9-BANK	72	0.0589	-7470A	PPB		26 Sep 2018 08:54:25	U	SMPL
CCV83 - 1	CCV83	14857	4.9846	-7470A	PPB		26 Sep 2018 08:56:32	U	SMPL
CCB83 - 1	CCB83	-247	-0.0474	-7470A	PPB		26 Sep 2018 08:58:39	U	SMPL
J5057-10 - 1	HC-SOIL	-25	0.0266	-7470A	PPB		26 Sep 2018 09:00:47	U	SMPL
J5059-04 - 1	PHASE-2	35	0.0466	-7470A	PPB		26 Sep 2018 09:02:55	U	SMPL
J5061-04 - 1	230-KV-A	12	0.0389	-7470A	PPB		26 Sep 2018 09:05:01	U	SMPL
J5061-09 - 1	230-KV-B	89	0.0646	-7470A	PPB		26 Sep 2018 09:07:09	U	SMPL
J5061-14 - 1	230-KV-C	57	0.0539	-7470A	PPB		26 Sep 2018 09:09:16	U	SMPL
J5061-14DUP - 1	230-KV-CDUP	-98	0.0023	-7470A	PPB		26 Sep 2018 09:11:26	U	SMPL
J5061-14MS - 1	230-KV-CMS	11114	3.7376	-7470A	PPB		26 Sep 2018 09:13:34	U	SMPL
J5061-14MSD - 1	230-KV-CMSD	11100	3.7329	-7470A	PPB		26 Sep 2018 09:15:44	U	SMPL
PB113169BL - 1	PBW	-64	0.0136	-7470A	PPB		26 Sep 2018 09:17:54	U	SMPL
PB113169BS - 1	LCSW	11551	3.8832	-7470A	PPB		26 Sep 2018 09:20:01	U	SMPL
CCV84 - 1	CCV84	15318	5.1382	-7470A	PPB		26 Sep 2018 09:22:09	U	SMPL
CCB84 - 1	CCB84	-260	-0.0517	-7470A	PPB		26 Sep 2018 09:24:18	U	SMPL
J5033-02 - 1	BPSI-TT-MW314D-20180919	-149	-0.0147	-7470A	PPB		26 Sep 2018 09:26:30	U	SMPL
J5033-02DUP - 1	BPSI-TT-MW314D-20180919DUP	36	0.0469	-7470A	PPB		26 Sep 2018 09:28:40	U	SMPL
J5033-02MS - 1	BPSI-TT-MW314D-20180919MS	11656	3.9182	-7470A	PPB		26 Sep 2018 09:30:47	U	SMPL
J5033-02MSD - 1	BPSI-TT-MW314D-20180919MSD	11757	3.9518	-7470A	PPB		26 Sep 2018 09:32:54	U	SMPL
J5033-03 - 1	BPSI-TT-MW301S-20180918	-129	-0.0081	-7470A	PPB		26 Sep 2018 09:35:02	U	SMPL
J5033-04 - 1	BB-TT-DUP05-20180918	-58	0.0156	-7470A	PPB		26 Sep 2018 09:37:10	U	SMPL
J5033-05 - 1	BP-HN-MW271-20180918	-8	0.0322	-7470A	PPB		26 Sep 2018 09:39:20	U	SMPL
J5033-06 - 1	BPSI-TT-MW301D-20180918	-82	0.0076	-7470A	PPB		26 Sep 2018 09:41:28	U	SMPL
J5033-07 - 1	BPSI-TT-MW301I-20180918	-119	-0.0047	-7470A	PPB		26 Sep 2018 09:43:40	U	SMPL
J5033-08 - 1	BP-MH-SW4001-20180918	119	0.0745	-7470A	PPB		26 Sep 2018 09:45:47	U	SMPL
CCV85 - 1	CCV85	15223	5.1065	-7470A	PPB		26 Sep 2018 09:47:54	U	SMPL
CCB85 - 1	CCB85	-116	-0.0037	-7470A	PPB		26 Sep 2018 09:50:02	U	SMPL
J5033-09 - 1	BP-TT-SW4004-20180918	125	0.0765	-7470A	PPB		26 Sep 2018 09:52:10	U	SMPL
J5033-10 - 1	BP-TT-SW4002-20180918	110	0.0716	-7470A	PPB		26 Sep 2018 09:54:18	U	SMPL
J5033-11 - 1	BPSI-TT-MW312I-20180918	124	0.0762	-7470A	PPB		26 Sep 2018 09:56:27	U	SMPL
J5033-12 - 1	BPSI-TT-MW312S-20180918	55	0.0532	-7470A	PPB		26 Sep 2018 09:58:34	U	SMPL
J5033-13 - 1	BPSI-TT-MW310S-20180919	95	0.0666	-7470A	PPB		26 Sep 2018 10:00:44	U	SMPL
J5033-14 - 1	BPSI-TT-MW311S-20180919	67	0.0572	-7470A	PPB		26 Sep 2018 10:02:53	U	SMPL
J5033-15 - 1	BPSI-TT-MW311I-20180919	73	0.0592	-7470A	PPB		26 Sep 2018 10:05:01	U	SMPL
J5033-18 - 1	BPSI-TT-MW314S-20180919	131	0.0785	-7470A	PPB		26 Sep 2018 10:07:10	U	SMPL
J5033-20 - 1	BPSI-TT-MW313S-20180920	77	0.0606	-7470A	PPB		26 Sep 2018 10:09:18	U	SMPL
J5033-21 - 1	BB-TT-DUP06-20180920	186	0.0969	-7470A	PPB		26 Sep 2018 10:11:26	U	SMPL
CCV86 - 1	CCV86	14527	4.8746	-7470A	PPB		26 Sep 2018 10:13:33	U	SMPL
CCB86 - 1	CCB86	-174	-0.0231	-7470A	PPB		26 Sep 2018 10:15:44	U	SMPL
J5033-22 - 1	BPSI-TT-MW307D-2018020	8	0.0376	-7470A	PPB		26 Sep 2018 10:17:55	U	SMPL
J5056-01 - 1	RA-BASELINE-WATER	361	0.1552	-7470A	PPB		26 Sep 2018 10:20:03	U	SMPL
J5061-14LX5 - 1		-45	0.0199	-7470A	PPB		26 Sep 2018 10:22:10	U	SMPL
J5061-14A - 1		11044	3.7143	-7470A	PPB		26 Sep 2018 10:24:19	U	SMPL
J5033-02LX5 - 1		-143	-0.0127	-7470A	PPB		26 Sep 2018 10:26:28	U	SMPL
J5033-02A - 1		11818	3.9721	-7470A	PPB		26 Sep 2018 10:28:35	U	SMPL
CCV87 - 1	CCV87	15362	5.1528	-7470A	PPB		26 Sep 2018 10:30:44	U	SMPL
CCB87 - 1	CCB87	-264	-0.0530	-7470A	PPB		26 Sep 2018 10:32:53	U	SMPL