

LA98177


7470A

INSTRUMENT ID : CV2

Linear

μ Abs. :

35892

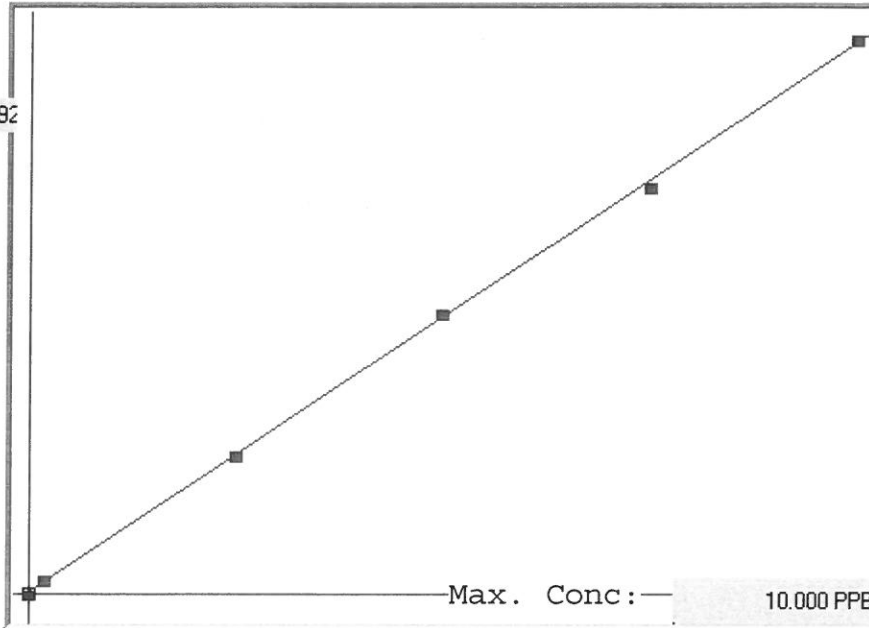

A= 0.0000e+000

B= 2.8103e-004

C= -3.2761e-002

Rho= 0.9998479

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.022	-0.022	38	0.000	38				
0.2	0.200	0.218	0.018	892	0.0 %	892				
2.5	2.500	2.502	0.002	9021	0.0 %	9021				
5.0	5.000	5.073	0.073	18168	0.0 %	18168				
7.5	7.500	7.374	-0.126	26357	0.0 %	26357				
10.0	10.000	10.054	0.054	35892	0.0 %	35892				

LB98177 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Sep 2018 10:10:26

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	38	-	0.0000	7470A	PPB	27 Sep 2018 10:17:10	S	Std
0.2 - 1	502	892	-	0.2000	7470A	PPB	27 Sep 2018 10:19:19	S	Std
2.5 - 1	52.5	9021	-	2.5000	7470A	PPB	27 Sep 2018 10:21:27	S	Std
5.0 - 1	55	18168	-	5.0000	7470A	PPB	27 Sep 2018 10:23:35	S	Std
7.5 - 1	59.5	26357	-	7.5000	7470A	PPB	27 Sep 2018 10:25:43	S	Std
10.0 - 1	511	35892	-	10.0000	7470A	PPB	27 Sep 2018 10:27:51	S	Std
ICV84 - 1	ICV84	14468	4.0333	-	7470A	PPB	27 Sep 2018 10:30:31	U	SMPL
ICB84 - 1	ICB84	-38	-0.0434	-	7470A	PPB	27 Sep 2018 10:32:37	U	SMPL
CCV01 - 1	CCV01	18202	5.0826	-	7470A	PPB	27 Sep 2018 10:34:45	U	SMPL
CCB01 - 1	CCB01	113	-0.0010	-	7470A	PPB	27 Sep 2018 10:39:17	U	SMPL
CRA - 1	CRA	822	0.1983	-	7470A	PPB	27 Sep 2018 10:41:23	U	SMPL
HighStd - 1	HighStd	35442	9.9277	-	7470A	PPB	27 Sep 2018 10:43:29	U	SMPL
ChkStd - 1	ChkStd	25096	7.0201	-	7470A	PPB	27 Sep 2018 10:50:09	U	SMPL
PB113259BL - 1	PBW	-19	-0.0381	-	7470A	PPB	27 Sep 2018 10:52:16	U	SMPL
PB113259BS - 1	LCSW	13583	3.7845	-	7470A	PPB	27 Sep 2018 10:54:25	U	SMPL
PB113259TB - 1	PB113218TB	101	-0.0044	-	7470A	PPB	27 Sep 2018 10:56:32	U	SMPL
J4773-12 - 1	CL-02-092518-A	282	0.0465	-	7470A	PPB	27 Sep 2018 10:58:41	U	SMPL
J4773-14 - 1	CL-02-092518-B	306	0.0532	-	7470A	PPB	27 Sep 2018 11:00:49	U	SMPL
J4773-16 - 1	CL-02-092518-C	146	0.0083	-	7470A	PPB	27 Sep 2018 11:02:58	U	SMPL
J4773-18 - 1	CL-02-092518-D	430	0.0881	-	7470A	PPB	27 Sep 2018 11:05:04	U	SMPL
CCV02 - 1	CCV02	18039	5.0368	-	7470A	PPB	27 Sep 2018 11:07:11	U	SMPL
CCB02 - 1	CCB02	-65	-0.0510	-	7470A	PPB	27 Sep 2018 11:09:17	U	SMPL
J4773-20 - 1	CL-02-092518-E	228	0.0313	-	7470A	PPB	27 Sep 2018 11:11:25	U	SMPL
J5074-10 - 1	CA-SOIL-1	344	0.0639	-	7470A	PPB	27 Sep 2018 11:13:32	U	SMPL
J5074-20 - 1	CA-SOIL-2	457	0.0957	-	7470A	PPB	27 Sep 2018 11:15:39	U	SMPL
J5081-04 - 1	TP-1-S	445	0.0923	-	7470A	PPB	27 Sep 2018 11:17:46	U	SMPL
J5081-08 - 1	TP-1-D	540	0.1190	-	7470A	PPB	27 Sep 2018 11:19:53	U	SMPL
J5081-12 - 1	TP-2-S	239	0.0344	-	7470A	PPB	27 Sep 2018 11:22:01	U	SMPL
J5081-12DUP - 1	TP-2-SDUP	277	0.0451	-	7470A	PPB	27 Sep 2018 11:24:09	U	SMPL
J5081-12MS - 1	TP-2-SMS	13389	3.7300	-	7470A	PPB	27 Sep 2018 11:26:17	U	SMPL
J5081-12MSD - 1	TP-2-SMSD	13186	3.6730	-	7470A	PPB	27 Sep 2018 11:28:26	U	SMPL
J5081-16 - 1	TP-2-D	182	0.0184	-	7470A	PPB	27 Sep 2018 11:30:34	U	SMPL
CCV03 - 1	CCV03	18178	5.0759	-	7470A	PPB	27 Sep 2018 11:32:42	U	SMPL
CCB03 - 1	CCB03	-51	-0.0471	-	7470A	PPB	27 Sep 2018 11:34:49	U	SMPL
PB113260BL - 1	PBW	174	0.0161	-	7470A	PPB	27 Sep 2018 11:40:04	U	SMPL
PB113260BS - 1	LCSW	12426	3.4594	-	7470A	PPB	27 Sep 2018 11:42:11	U	SMPL
PB113260TB - 1	PB113237TB	24	-0.0260	-	7470A	PPB	27 Sep 2018 11:44:18	U	SMPL
J5078-02 - 1	600-WILSON-AVE-NEWARK	309	0.0541	-	7470A	PPB	27 Sep 2018 11:46:25	U	SMPL
J5078-02DUP - 1	600-WILSON-AVE-NEWARKDUP	319	0.0569	-	7470A	PPB	27 Sep 2018 11:48:32	U	SMPL
J5078-02MS - 1	600-WILSON-AVE-NEWARKMS	14226	3.9652	-	7470A	PPB	27 Sep 2018 11:50:40	U	SMPL
J5078-02MSD - 1	600-WILSON-AVE-NEWARKMSD	13234	3.6865	-	7470A	PPB	27 Sep 2018 11:52:48	U	SMPL
J5085-08 - 1	MH-720	194	0.0218	-	7470A	PPB	27 Sep 2018 11:54:57	U	SMPL
J5085-09 - 1	MH-719	270	0.0431	-	7470A	PPB	27 Sep 2018 11:57:06	U	SMPL
J5085-10 - 1	MH-717	264	0.0414	-	7470A	PPB	27 Sep 2018 11:59:13	U	SMPL
CCV04 - 1	CCV04	18301	5.1105	-	7470A	PPB	27 Sep 2018 12:01:20	U	SMPL
CCB04 - 1	CCB04	108	-0.0024	-	7470A	PPB	27 Sep 2018 12:03:28	U	SMPL
J5085-11 - 1	MH-10.25	214	0.0274	-	7470A	PPB	27 Sep 2018 12:05:35	U	SMPL
J5085-12 - 1	MH-10.29	369	0.0709	-	7470A	PPB	27 Sep 2018 12:07:43	U	SMPL
J5085-13 - 1	MH-714	266	0.0420	-	7470A	PPB	27 Sep 2018 12:09:50	U	SMPL
J5085-14 - 1	MH-713	108	-0.0024	-	7470A	PPB	27 Sep 2018 12:11:57	U	SMPL
PB113261BL - 1	PBW	250	0.0375	-	7470A	PPB	27 Sep 2018 12:14:04	U	SMPL
PB113261BS - 1	LCSW	13479	3.7553	-	7470A	PPB	27 Sep 2018 12:16:12	U	SMPL
J5078-01 - 1	600-WILSON-AVE-NEWARK	1229	0.3126	-	7470A	PPB	27 Sep 2018 12:18:20	U	SMPL
J5085-01 - 1	MH-720	707	0.1659	-	7470A	PPB	27 Sep 2018 12:28:10	U	SMPL
J5085-01DUP - 1	MH-720DUP	671	0.1558	-	7470A	PPB	27 Sep 2018 12:30:17	U	SMPL
J5085-01MS - 1	MH-720MS	14488	4.0389	-	7470A	PPB	27 Sep 2018 12:32:25	U	SMPL
CCV05 - 1	CCV05	18304	5.1113	-	7470A	PPB	27 Sep 2018 12:34:32	U	SMPL
CCB05 - 1	CCB05	110	-0.0018	-	7470A	PPB	27 Sep 2018 12:36:40	U	SMPL
J5085-01MSD - 1	MH-720MSD	14320	3.9917	-	7470A	PPB	27 Sep 2018 12:38:49	U	SMPL
J5085-02 - 1	MH-719	1440	0.3719	-	7470A	PPB	27 Sep 2018 12:40:56	U	SMPL
J5085-03 - 1	MH-717	1984	0.5248	-	7470A	PPB	27 Sep 2018 12:43:06	U	SMPL
J5085-04 - 1	MH-10.25	716	0.1685	-	7470A	PPB	27 Sep 2018 12:45:13	U	SMPL
J5085-05 - 1	MH-10.29	304	0.0527	-	7470A	PPB	27 Sep 2018 12:47:21	U	SMPL
J5085-06 - 1	MH-714	335	0.0614	-	7470A	PPB	27 Sep 2018 12:49:28	U	SMPL
J5085-07 - 1	MH-713	552	0.1224	-	7470A	PPB	27 Sep 2018 12:51:36	U	SMPL
PB113280BL - 1	PBW	-17	-0.0375	-	7470A	PPB	27 Sep 2018 12:53:45	U	SMPL
PB113280BS - 1	LCSW	12932	3.6016	-	7470A	PPB	27 Sep 2018 12:55:53	U	SMPL
J5033-24 - 1	BPSI-TT-MW314D-20180919	-43	-0.0448	-	7470A	PPB	27 Sep 2018 12:58:01	U	SMPL
CCV06 - 1	CCV06	18468	5.1574	-	7470A	PPB	27 Sep 2018 13:00:09	U	SMPL
CCB06 - 1	CCB06	152	0.0100	-	7470A	PPB	27 Sep 2018 13:02:17	U	SMPL
J5033-24DUP - 1	BPSI-TT-MW314D-20180919DUP	-34	-0.0423	-	7470A	PPB	27 Sep 2018 13:04:25	U	SMPL
J5033-24MS - 1	BPSI-TT-MW314D-20180919MS	13314	3.7089	-	7470A	PPB	27 Sep 2018 13:06:33	U	SMPL
J5033-24MSD - 1	BPSI-TT-MW314D-20180919MSD	13381	3.7278	-	7470A	PPB	27 Sep 2018 13:08:40	U	SMPL
J5033-25 - 1	BPSI-TT-MW301S-20180918	-109	-0.0634	-	7470A	PPB	27 Sep 2018 13:10:47	U	SMPL
J5033-26 - 1	BB-TT-DUP05-20180918	14	-0.0288	-	7470A	PPB	27 Sep 2018 13:12:54	U	SMPL
J5033-27 - 1	BP-HN-MW27I-20180918	40	-0.0215	-	7470A	PPB	27 Sep 2018 13:15:02	U	SMPL
J5033-28 - 1	BPSI-TT-MW301D-20180918	81	-0.0100	-	7470A	PPB	27 Sep 2018 13:17:10	U	SMPL
J5033-29 - 1	BPSI-TT-MW301I-20180918	21	-0.0269	-	7470A	PPB	27 Sep 2018 13:19:18	U	SMPL
J5033-30 - 1	BP-MH-SW400I-20180918	31	-0.0240	-	7470A	PPB	27 Sep 2018 13:21:26	U	SMPL
J5033-31 - 1	BP-TT-SW400A-20180918	65	-0.0145	-	7470A	PPB	27 Sep 2018 13:23:34	U	SMPL
CCV07 - 1	CCV07	18165	5.0722	-	7470A	PPB	27 Sep 2018 13:25:42	U	SMPL
CCB07 - 1	CCB07	-116	-0.0654	-	7470A	PPB	27 Sep 2018 13:27:50	U	SMPL
J5033-32 - 1	BP-TT-SW4002-20180918	111	-0.0016	-	7470A	PPB	27 Sep 2018 13:29:58	U	SMPL
J5033-33 - 1	BPSI-TT-MW312I-20180918	-6	-0.0344	-	7470A	PPB	27 Sep 2018 13:32:06	U	SMPL
J5033-34 - 1	BPSI-TT-MW312S-20180918	17	-0.0280	-	7470A	PPB	27 Sep 2018 13:34:14	U	SMPL
J5033-35 - 1	BPSI-TT-MW310S-20180919	3	-0.0319	-	7470A	PPB	27 Sep 2018 13:36:21	U	SMPL
J5033-36 - 1	BPSI-TT-MW311S-20180919	26	-0.0255	-	7470A	PPB	27 Sep 2018 13:38:29	U	SMPL
J5033-37 - 1	BPSI-TT-MW311I-20180919	59	-0.0162	-	7470A	PPB	27 Sep 2018 13:40:37	U	SMPL
J5033-38 - 1	BPSI-TT-MW314S-20180919	15	-0.0285	-	7470A	PPB	27 Sep 2018 13:42:45	U	SMPL
J5033-39 - 1	BPSI-TT-MW313S-20180920	33	-0.0235	-	7470A	PPB	27 Sep 2018 13:44:53	U	SMPL
J5033-40 - 1	BB-TT-DUP06-20180920	14	-0.0288	-	7470A	PPB	27 Sep 2018 13:47:02	U	SMPL
J5033-41 - 1	BPSI-TT-MW307D-20180920	13	-0.0291	-	7470A	PPB	27 Sep 2018 13:49:10	U	SMPL
CCV08 - 1	CCV08	17657	4.9295	-	7470A	PPB	27 Sep 2018 13:51:17	U	SMPL

LB98177 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Sep 2018 10:10:26

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
CCB08 - 1	CCB08	26	-0.0255		-7470A	PPB	27 Sep 2018 13:56:48	U	SMPL
J5081-12LX5 - 1		58	-0.0165		-7470A	PPB	27 Sep 2018 13:58:55	U	SMPL
J5081-12A - 1		14739	4.1094		-7470A	PPB	27 Sep 2018 14:01:03	U	SMPL
J5078-02LX5 - 1		-21	-0.0387		-7470A	PPB	27 Sep 2018 14:03:11	U	SMPL
J5078-02A - 1		14920	4.1603		-7470A	PPB	27 Sep 2018 14:05:18	U	SMPL
J5085-01LX5 - 1		30	-0.0243		-7470A	PPB	27 Sep 2018 14:07:26	U	SMPL
J5085-01A - 1		15526	4.3306		-7470A	PPB	27 Sep 2018 14:09:34	U	SMPL
J5033-24LX5 - 1		-153	-0.0758		-7470A	PPB	27 Sep 2018 14:11:42	U	SMPL
J5033-24A - 1		14271	3.9779		-7470A	PPB	27 Sep 2018 14:13:52	U	SMPL
CCV09 - 1	CCV09	18098	5.0534		-7470A	PPB	27 Sep 2018 14:16:01	U	SMPL
CCB09 - 1	CCB09	43	-0.0207		-7470A	PPB	27 Sep 2018 14:18:10	U	SMPL