

LB 98230


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

37308

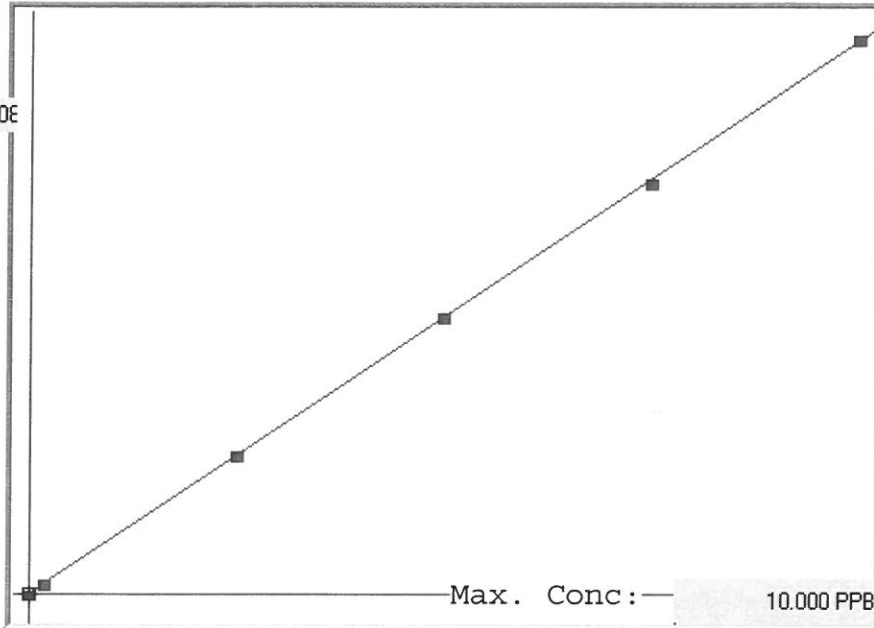

A= 0.0000e+000

B= 2.6900e-004

C= -9.6588e-003

Rho= 0.9999764

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.011	0.011	75	0.000	75				
0.2	0.200	0.192	-0.008	748	0.0 %	748				
2.5	2.500	2.499	-0.001	9326	0.0 %	9326				
5.0	5.000	5.023	0.023	18708	0.0 %	18708				
7.5	7.500	7.450	-0.050	27732	0.0 %	27732				
10.0	10.000	10.026	0.026	37308	0.0 %	37308				

LB98230 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Sep 2018 14:44:30

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	75	-	0.0000	7470A	PPB	28 Sep 2018 14:46:44	S	Std
0.2 - 1	50.2	748	-	0.2000	7470A	PPB	28 Sep 2018 14:48:52	S	Std
2.5 - 1	52.5	9326	-	2.5000	7470A	PPB	28 Sep 2018 14:51:00	S	Std
5.0 - 1	55	18708	-	5.0000	7470A	PPB	28 Sep 2018 14:53:08	S	Std
7.5 - 1	57.5	27732	-	7.5000	7470A	PPB	28 Sep 2018 14:55:16	S	Std
10.0 - 1	510	37308	-	10.0000	7470A	PPB	28 Sep 2018 15:00:13	S	Std
ICV88 - 1	ICV88	14683	3.9400	-7470A	PPB	PPB	28 Sep 2018 15:03:10	U	SMPL
ICB88 - 1	ICB88	-107	-0.0384	-7470A	PPB	PPB	28 Sep 2018 15:05:16	U	SMPL
CCV28 - 1	CCV28	19039	5.1118	-7470A	PPB	PPB	28 Sep 2018 15:07:25	U	SMPL
CCB28 - 1	CCB28	-87	-0.0331	-7470A	PPB	PPB	28 Sep 2018 15:09:31	U	SMPL
CRA - 1	CRA	765	0.1961	-7470A	PPB	PPB	28 Sep 2018 15:11:39	U	SMPL
HighStd - 1	HighStd	37847	10.1710	-7470A	PPB	PPB	28 Sep 2018 15:13:45	U	SMPL
ChkStd - 1	ChkStd	25684	6.8992	-7470A	PPB	PPB	28 Sep 2018 15:15:52	U	SMPL
PB113315BL - 1	PBW	-170	-0.0554	-7470A	PPB	PPB	28 Sep 2018 15:18:01	U	SMPL
PB113315BS - 1	LCSW	14593	3.9158	-7470A	PPB	PPB	28 Sep 2018 15:22:47	U	SMPL
PB113315TB - 1	PB113262TB	7	-0.0078	-7470A	PPB	PPB	28 Sep 2018 15:24:55	U	SMPL
J5096-02 - 1	MT-T-5-2	156	0.0323	-7470A	PPB	PPB	28 Sep 2018 15:27:04	U	SMPL
J5096-02DUP - 1	MT-T-5-2DUP	155	0.0320	-7470A	PPB	PPB	28 Sep 2018 15:29:13	U	SMPL
J5096-02MS - 1	MT-T-5-2MS	13579	3.6430	-7470A	PPB	PPB	28 Sep 2018 15:31:21	U	SMPL
J5096-02MSD - 1	MT-T-5-2MSD	13222	3.5470	-7470A	PPB	PPB	28 Sep 2018 15:33:28	U	SMPL
CCV29 - 1	CCV29	18335	4.9224	-7470A	PPB	PPB	28 Sep 2018 15:35:35	U	SMPL
CCB29 - 1	CCB29	-131	-0.0449	-7470A	PPB	PPB	28 Sep 2018 15:37:43	U	SMPL
J5097-02 - 1	TP-1	226	0.0511	-7470A	PPB	PPB	28 Sep 2018 15:39:51	U	SMPL
J5097-04 - 1	TP-2	96	0.0162	-7470A	PPB	PPB	28 Sep 2018 15:41:58	U	SMPL
J5097-06 - 1	TP-3	116	0.0215	-7470A	PPB	PPB	28 Sep 2018 15:44:05	U	SMPL
J5097-08 - 1	TP-4	78	0.0113	-7470A	PPB	PPB	28 Sep 2018 15:46:12	U	SMPL
J5099-02 - 1	7211975	295	0.0697	-7470A	PPB	PPB	28 Sep 2018 15:48:19	U	SMPL
J5100-04 - 1	HS-STONE-RO-227	318	0.0759	-7470A	PPB	PPB	28 Sep 2018 15:50:27	U	SMPL
PB113316BL - 1	PBW	147	0.0299	-7470A	PPB	PPB	28 Sep 2018 15:52:34	U	SMPL
PB113316BS - 1	LCSW	14690	3.9419	-7470A	PPB	PPB	28 Sep 2018 15:54:43	U	SMPL
PB113316TB - 1	PB113264TB	29	-0.0019	-7470A	PPB	PPB	28 Sep 2018 15:56:51	U	SMPL
J5101-02 - 1	C-1329	133	0.0261	-7470A	PPB	PPB	28 Sep 2018 15:58:59	U	SMPL
CCV30 - 1	CCV30	18347	4.9256	-7470A	PPB	PPB	28 Sep 2018 16:01:06	U	SMPL
CCB30 - 1	CCB30	-118	-0.0414	-7470A	PPB	PPB	28 Sep 2018 16:03:13	U	SMPL
J5101-02DUP - 1	C-1329DUP	119	0.0224	-7470A	PPB	PPB	28 Sep 2018 16:05:21	U	SMPL
J5101-02MS - 1	C-1329MS	13290	3.5653	-7470A	PPB	PPB	28 Sep 2018 16:07:28	U	SMPL
J5101-02MSD - 1	C-1329MSD	13653	3.6629	-7470A	PPB	PPB	28 Sep 2018 16:09:35	U	SMPL
PB113317BL - 1	PBW	1	-0.0094	-7470A	PPB	PPB	28 Sep 2018 16:11:44	U	SMPL
PB113317BS - 1	LCSW	14781	3.9664	-7470A	PPB	PPB	28 Sep 2018 16:13:52	U	SMPL
J5101-01 - 1	C-1329	42	0.0016	-7470A	PPB	PPB	28 Sep 2018 16:15:59	U	SMPL
J5101-01DUP - 1	C-1329DUP	167	0.0353	-7470A	PPB	PPB	28 Sep 2018 16:18:08	U	SMPL
J5101-01MS - 1	C-1329MS	13317	3.5726	-7470A	PPB	PPB	28 Sep 2018 16:20:16	U	SMPL
J5101-01MSD - 1	C-1329MSD	13807	3.7044	-7470A	PPB	PPB	28 Sep 2018 16:22:25	U	SMPL
CCV31 - 1	CCV31	18744	5.0324	-7470A	PPB	PPB	28 Sep 2018 16:24:33	U	SMPL
CCB31 - 1	CCB31	-87	-0.0331	-7470A	PPB	PPB	28 Sep 2018 16:26:41	U	SMPL
J5096-02LX5 - 1		84	0.0129	-7470A	PPB	PPB	28 Sep 2018 16:28:49	U	SMPL
J5096-02A - 1		15095	4.0508	-7470A	PPB	PPB	28 Sep 2018 16:30:56	U	SMPL
J5101-02LX5 - 1		-95	-0.0352	-7470A	PPB	PPB	28 Sep 2018 16:33:03	U	SMPL
J5101-02A - 1		14850	3.9849	-7470A	PPB	PPB	28 Sep 2018 16:35:11	U	SMPL
J5101-01LX5 - 1		-51	-0.0234	-7470A	PPB	PPB	28 Sep 2018 16:37:18	U	SMPL
J5101-01A - 1		15194	4.0775	-7470A	PPB	PPB	28 Sep 2018 16:39:26	U	SMPL
CCV32 - 1	CCV32	18326	4.9200	-7470A	PPB	PPB	28 Sep 2018 16:41:34	U	SMPL
CCB32 - 1	CCB32	-86	-0.0328	-7470A	PPB	PPB	28 Sep 2018 16:43:42	U	SMPL