


7470A

LB 98896
INSTRUMENT ID: CV1

Linear

 μ Abs.:

34401

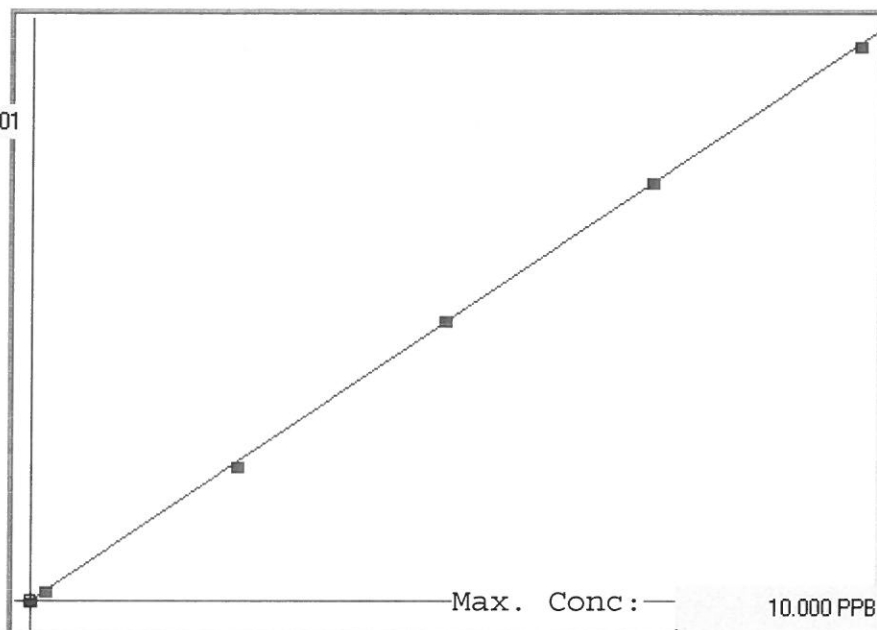

A= 0.0000e+000

B= 2.8925e-004

C= 7.7493e-003

Rho= 0.9999400

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.013	0.013	19	0.000	19				
0.2	0.200	0.194	-0.006	645	0.0 %	645				
2.5	2.500	2.442	-0.058	8415	0.0 %	8415				
5.0	5.000	5.055	0.055	17451	0.0 %	17451				
7.5	7.500	7.537	0.037	26031	0.0 %	26031				
10.0	10.000	9.958	-0.042	34401	0.0 %	34401				

LB98396 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Oct 2018 10:03:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	19	-	0.0000	7470A	PPB	05 Oct 2018 10:16:29	S	Std
0.2 - 1	50.2	645	-	0.2000	7470A	PPB	05 Oct 2018 10:18:38	S	Std
2.5 - 1	52.5	8415	-	2.5000	7470A	PPB	05 Oct 2018 10:20:47	S	Std
5.0 - 1	55	17451	-	5.0000	7470A	PPB	05 Oct 2018 10:22:55	S	Std
7.5 - 1	57.5	26031	-	7.5000	7470A	PPB	05 Oct 2018 10:25:04	S	Std
10.0 - 1	510	34401	-	10.0000	7470A	PPB	05 Oct 2018 10:27:12	S	Std
ICV05 - 1	ICV05	13271	3.8463	-7470A	PPB	PPB	05 Oct 2018 10:29:47	U	SMPL
ICB05 - 1	ICB05	-110	-0.0241	-7470A	PPB	PPB	05 Oct 2018 10:31:55	U	SMPL
CCV94 - 1	CCV94	18237	5.2827	-7470A	PPB	PPB	05 Oct 2018 10:34:02	U	SMPL
CCB94 - 1	CCB94	-56	-0.0084	-7470A	PPB	PPB	05 Oct 2018 10:36:09	U	SMPL
CRA - 1	CRA	677	0.2036	-7470A	PPB	PPB	05 Oct 2018 10:38:17	U	SMPL
HighStd - 1	HighStd	34977	10.1247	-7470A	PPB	PPB	05 Oct 2018 10:40:24	U	SMPL
ChkStd - 1	ChkStd	24483	7.0894	-7470A	PPB	PPB	05 Oct 2018 10:42:31	U	SMPL
PB113529BL - 1	PBW	-230	-0.0588	-7470A	PPB	PPB	05 Oct 2018 10:44:41	U	SMPL
PB113529BS - 1	LCSW	13450	3.8981	-7470A	PPB	PPB	05 Oct 2018 10:46:51	U	SMPL
PB113529TB - 1	PB113486TB	-92	-0.0189	-7470A	PPB	PPB	05 Oct 2018 10:48:58	U	SMPL
J5199-02 - 1	OK-01-100318	59	0.0248	-7470A	PPB	PPB	05 Oct 2018 10:51:07	U	SMPL
J5204-02 - 1	SU-04-100318-A	75	0.0294	-7470A	PPB	PPB	05 Oct 2018 10:53:17	U	SMPL
J5204-02DUP - 1	SU-04-100318-ADUP	90	0.0338	-7470A	PPB	PPB	05 Oct 2018 10:55:26	U	SMPL
J5204-02MS - 1	SU-04-100318-AMS	11606	3.3648	-7470A	PPB	PPB	05 Oct 2018 10:57:33	U	SMPL
CCV95 - 1	CCV95	18306	5.3027	-7470A	PPB	PPB	05 Oct 2018 10:59:41	U	SMPL
CCB95 - 1	CCB95	-137	-0.0319	-7470A	PPB	PPB	05 Oct 2018 11:01:48	U	SMPL
J5204-02MSD - 1	SU-04-100318-AMSD	12266	3.5557	-7470A	PPB	PPB	05 Oct 2018 11:03:57	U	SMPL
J5204-04 - 1	SU-04-100318-B	-81	-0.0157	-7470A	PPB	PPB	05 Oct 2018 11:06:04	U	SMPL
J5238-03 - 1	MT-T-5-8	55	0.0237	-7470A	PPB	PPB	05 Oct 2018 11:08:11	U	SMPL
J5244-01 - 1	OILY-DEBRIS-A	-92	-0.0189	-7470A	PPB	PPB	05 Oct 2018 11:10:18	U	SMPL
J5244-02 - 1	OILY-DEBRIS-B	75	0.0294	-7470A	PPB	PPB	05 Oct 2018 11:12:25	U	SMPL
J5244-03 - 1	OIL	-53	-0.0076	-7470A	PPB	PPB	05 Oct 2018 11:14:33	U	SMPL
J5204-02LX5 - 1		10	0.0106	-7470A	PPB	PPB	05 Oct 2018 11:16:41	U	SMPL
J5204-02A - 1		13180	3.8200	-7470A	PPB	PPB	05 Oct 2018 11:22:57	U	SMPL
CCV96 - 1	CCV96	17703	5.1283	-7470A	PPB	PPB	05 Oct 2018 11:25:07	U	SMPL
CCB96 - 1	CCB96	-103	-0.0220	-7470A	PPB	PPB	05 Oct 2018 11:27:14	U	SMPL