

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

10/5/2018 11:54

Test: *Reactive*
~~Total~~ CN *ug/d*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.736	0.0	0.084	
ICB1	-0.055	0.0	0.004	
CCV1	240.592	0.0	0.205	
CCB1	-0.430	0.0	0.003	
PB113561BL	0.051	0.0	0.004	
J5179-04	-0.348	0.0	0.003	
J5179-04DUP	-0.494	0.0	0.003	
J5179-08	-0.716	0.0	0.003	
J5195-02	-0.888	0.0	0.003	
J5205-02	-0.669	0.0	0.003	
J5255-06	5.832	0.0	0.008	
PB113562BL	-0.369	0.0	0.003	
J5248-02	1.181	0.0	0.005	
CCV2	243.965	0.0	0.208	
CCB2	-0.004	0.0	0.004	
J5248-02DUP	-0.221	0.0	0.003	
J5262-03	-0.001	0.0	0.004	
J5255-03	-0.607	0.0	0.003	
CCV3	255.870	0.0	0.218	
CCB3	0.153	0.0	0.004	

N 20
Mean 41.929
SD 90.8776
CV% 216.74

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

10/5/2018 11:05


Test Total CN

Accepted 10/5/2018 11:05

Factor 1194
 Bias 0.004

Coeff. of det. 0.999980

Errors

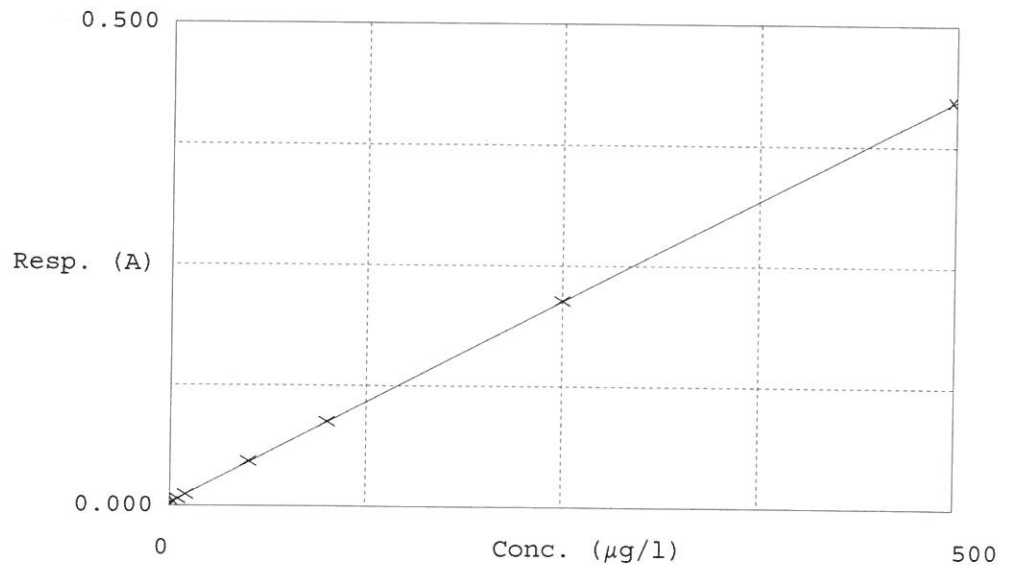

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.7241	0.0000	
2	5.0PPBCN	0.007	4.0949	5.0000	
3	10PPBCN	0.012	9.7831	10.0000	
4	50PPBCN	0.046	51.2417	50.0000	
5	100PPBCN	0.088	100.3844	100.0000	
6	250PPBCN	0.214	250.8153	250.0000	
7	500PPBCN	0.422	499.4047	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri Oct 05 10:47:05 2018

Fri Oct 05 11:53:38 2018

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.7241	µg/l	10/5/2018 10:47:05	
5.OPPBCN	A	Reactive CN	P	4.0949	µg/l	10/5/2018 10:47:06	
10PPBCN	A	Reactive CN	P	9.7831	µg/l	10/5/2018 10:47:07	
50PPBCN	A	Reactive CN	P	51.2417	µg/l	10/5/2018 10:47:08	
100PPBCN	A	Reactive CN	P	100.3844	µg/l	10/5/2018 10:47:09	
250PPBCN	A	Reactive CN	P	250.8153	µg/l	10/5/2018 10:47:10	
500PPBCN	A	Reactive CN	P	499.4047	µg/l	10/5/2018 10:47:11	
ICV1	S	Reactive CN	P	95.7357	µg/l	10/5/2018 11:31:19	
ICB1	S	Reactive CN	P	-0.055	µg/l	10/5/2018 11:31:20	
CCV1	S	Reactive CN	P	240.5919	µg/l	10/5/2018 11:31:21	
CCB1	S	Reactive CN	P	-0.4303	µg/l	10/5/2018 11:31:22	
PB113561BL	S	Reactive CN	P	0.051	µg/l	10/5/2018 11:31:23	
J5179-04	S	Reactive CN	P	-0.3476	µg/l	10/5/2018 11:31:24	
J5179-04DUP	S	Reactive CN	P	-0.4942	µg/l	10/5/2018 11:31:25	
J5179-08	S	Reactive CN	P	-0.7161	µg/l	10/5/2018 11:31:26	
J5195-02	S	Reactive CN	P	-0.8879	µg/l	10/5/2018 11:31:27	
J5205-02	S	Reactive CN	P	-0.6693	µg/l	10/5/2018 11:31:28	
J5255-06	S	Reactive CN	P	5.8323	µg/l	10/5/2018 11:37:58	
PB113562BL	S	Reactive CN	P	-0.3691	µg/l	10/5/2018 11:37:59	
J5248-02	S	Reactive CN	P	1.1809	µg/l	10/5/2018 11:38:00	
CCV2	S	Reactive CN	P	243.9647	µg/l	10/5/2018 11:38:01	
CCB2	S	Reactive CN	P	-0.004	µg/l	10/5/2018 11:38:02	
J5248-02DUP	S	Reactive CN	P	-0.2212	µg/l	10/5/2018 11:38:03	
J5262-03	S	Reactive CN	P	-0.0009	µg/l	10/5/2018 11:38:04	
J5255-03	S	Reactive CN	P	-0.6066	µg/l	10/5/2018 11:53:36	
CCV3	S	Reactive CN	P	255.8705	µg/l	10/5/2018 11:53:37	
CCB3	S	Reactive CN	P	0.1525	µg/l	10/5/2018 11:53:38	