


7470A

LB 98604
INSTRUMENT ID: CV1

Linear

 μ Abs.:

40637

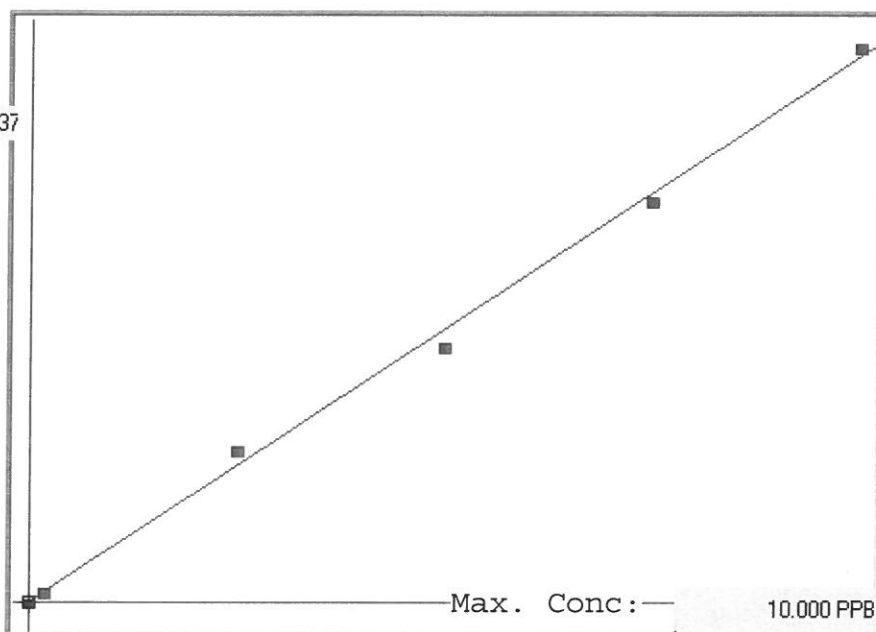

A= 0.0000e+000

B= 2.5010e-004

C= -1.0363e-003

Rho= 0.9986807

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	25	0.000	25				
0.2	0.200	0.182	-0.018	732	0.0 %	732				
2.5	2.500	2.788	0.288	11151	0.0 %	11151				
5.0	5.000	4.710	-0.290	18835	0.0 %	18835				
7.5	7.500	7.353	-0.147	29405	0.0 %	29405				
10.0	10.000	10.162	0.162	40637	0.0 %	40637				

LB98604 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Oct 2018 11:36:16

Sample ID	Extended ID	μ Abs	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	25	-	0.0000	7470A	PPB	15 Oct 2018 11:36:26	S	Std
0.2 - 1	50.2	732	-	0.2000	7470A	PPB	15 Oct 2018 11:38:34	S	Std
2.5 - 1	52.5	11151	-	2.5000	7470A	PPB	15 Oct 2018 11:40:43	S	Std
5.0 - 1	55	18835	-	5.0000	7470A	PPB	15 Oct 2018 11:42:51	S	Std
7.5 - 1	57.5	29405	-	7.5000	7470A	PPB	15 Oct 2018 11:47:31	S	Std
10.0 - 1	510	40637	-	10.0000	7470A	PPB	15 Oct 2018 11:52:05	S	Std
ICV22 - 1	ICV22	14418	3.6049	-	7470A	PPB	15 Oct 2018 11:55:00	U	SMPL
ICB22 - 1	ICB22	-52	-0.0140	-	7470A	PPB	15 Oct 2018 11:57:06	U	SMPL
CCV82 - 1	CCV82	19606	4.9024	-	7470A	PPB	15 Oct 2018 11:59:16	U	SMPL
CCB82 - 1	CCB82	-66	-0.0175	-	7470A	PPB	15 Oct 2018 12:01:22	U	SMPL
CRA - 1	CRA	761	0.1893	-	7470A	PPB	15 Oct 2018 12:03:30	U	SMPL
HighStd - 1	HighStd	39821	9.9582	-	7470A	PPB	15 Oct 2018 12:05:37	U	SMPL
ChkStd - 1	ChkStd	28101	7.0270	-	7470A	PPB	15 Oct 2018 12:10:37	U	SMPL
PB113817BL - 1	PBW	-273	-0.0693	-	7470A	PPB	15 Oct 2018 12:12:44	U	SMPL
PB113817BS - 1	LCSW	13226	3.3068	-	7470A	PPB	15 Oct 2018 12:14:52	U	SMPL
PB113817TB - 1	PB113778TB	-75	-0.0198	-	7470A	PPB	15 Oct 2018 12:17:00	U	SMPL
J5193-02 - 1	BU-01-101118	-5	-0.0023	-	7470A	PPB	15 Oct 2018 12:19:10	U	SMPL
J5193-02DUP - 1	BU-01-101118DUP	17	0.0032	-	7470A	PPB	15 Oct 2018 12:21:18	U	SMPL
J5193-02MS - 1	BU-01-101118MS	14756	3.6894	-	7470A	PPB	15 Oct 2018 12:25:48	U	SMPL
J5193-02MSD - 1	BU-01-101118MSD	14428	3.6074	-	7470A	PPB	15 Oct 2018 12:27:54	U	SMPL
CCV83 - 1	CCV83	19223	4.8066	-	7470A	PPB	15 Oct 2018 12:30:01	U	SMPL
CCB83 - 1	CCB83	-105	-0.0273	-	7470A	PPB	15 Oct 2018 12:32:07	U	SMPL
J5197-02 - 1	HD-01-101118	-21	-0.0063	-	7470A	PPB	15 Oct 2018 12:34:16	U	SMPL
J5199-04 - 1	OK-02-101118	38	0.0085	-	7470A	PPB	15 Oct 2018 12:36:23	U	SMPL
J5205-04 - 1	TR-04-101118	10	0.0015	-	7470A	PPB	15 Oct 2018 12:38:30	U	SMPL
J5392-02 - 1	SOIL-DRUM	-8	-0.0030	-	7470A	PPB	15 Oct 2018 12:40:37	U	SMPL
J5395-02 - 1	PH-SOIL	187	0.0457	-	7470A	PPB	15 Oct 2018 12:42:44	U	SMPL
J5450-03 - 1	VNJ218-210-282	1	-0.0008	-	7470A	PPB	15 Oct 2018 12:44:52	U	SMPL
J5450-04 - 1	MATTING	23	0.0047	-	7470A	PPB	15 Oct 2018 12:47:00	U	SMPL
J5455-03 - 1	MS-OILY-DEBRI	15	0.0027	-	7470A	PPB	15 Oct 2018 12:49:08	U	SMPL
J5457-03 - 1	KG-SOIL	54	0.0125	-	7470A	PPB	15 Oct 2018 12:51:17	U	SMPL
PB113818BL - 1	PBW	12	0.0020	-	7470A	PPB	15 Oct 2018 12:53:24	U	SMPL
CCV84 - 1	CCV84	18659	4.6656	-	7470A	PPB	15 Oct 2018 12:55:30	U	SMPL
CCB84 - 1	CCB84	-66	-0.0175	-	7470A	PPB	15 Oct 2018 12:57:37	U	SMPL
PB113818BS - 1	LCSW	14468	3.6174	-	7470A	PPB	15 Oct 2018 12:59:46	U	SMPL
PB113818TB - 1	PB113782TB	-40	-0.0110	-	7470A	PPB	15 Oct 2018 13:01:53	U	SMPL
J5455-06 - 1	MS-OILY-WATER	11	0.0017	-	7470A	PPB	15 Oct 2018 13:04:01	U	SMPL
J5455-06DUP - 1	MS-OILY-WATERDUP	3	-0.0003	-	7470A	PPB	15 Oct 2018 13:06:08	U	SMPL
J5455-06MS - 1	MS-OILY-WATERMS	16913	4.2289	-	7470A	PPB	15 Oct 2018 13:08:15	U	SMPL
J5455-06MSD - 1	MS-OILY-WATERMSD	16832	4.2086	-	7470A	PPB	15 Oct 2018 13:10:23	U	SMPL
J5456-02 - 1	MS-FRAC-TANK	-40	-0.0110	-	7470A	PPB	15 Oct 2018 13:12:30	U	SMPL
PB113819BL - 1	PBW	-3	-0.0018	-	7470A	PPB	15 Oct 2018 13:14:39	U	SMPL
PB113819BS - 1	LCSW	16869	4.2179	-	7470A	PPB	15 Oct 2018 13:16:47	U	SMPL
J5393-12 - 1	WE13-GW-TANK3-IDW-10102018	-197	-0.0503	-	7470A	PPB	15 Oct 2018 13:18:55	U	SMPL
CCV85 - 1	CCV85	19023	4.7566	-	7470A	PPB	15 Oct 2018 13:21:02	U	SMPL
CCB85 - 1	CCB85	-186	-0.0476	-	7470A	PPB	15 Oct 2018 13:23:09	U	SMPL
J5455-05 - 1	MS-OILY-WATER	40	0.0090	-	7470A	PPB	15 Oct 2018 13:31:03	U	SMPL
J5455-05DUP - 1	MS-OILY-WATERDUP	38	0.0085	-	7470A	PPB	15 Oct 2018 13:33:10	U	SMPL
J5455-05MS - 1	MS-OILY-WATERMS	14037	3.5096	-	7470A	PPB	15 Oct 2018 13:38:09	U	SMPL
J5455-05MSD - 1	MS-OILY-WATERMSD	13809	3.4526	-	7470A	PPB	15 Oct 2018 13:40:16	U	SMPL
J5456-01 - 1	MS-FRAC-TANK	752	0.1870	-	7470A	PPB	15 Oct 2018 13:42:23	U	SMPL
CCV86 - 1	CCV86	19276	4.8199	-	7470A	PPB	15 Oct 2018 13:54:21	U	SMPL
CCB86 - 1	CCB86	-174	-0.0446	-	7470A	PPB	15 Oct 2018 13:56:28	U	SMPL
J5193-02LX5 - 1		38	0.0085	-	7470A	PPB	15 Oct 2018 13:58:37	U	SMPL
J5193-02A - 1		13402	3.3508	-	7470A	PPB	15 Oct 2018 14:00:46	U	SMPL
J5455-06LX5 - 1		-65	-0.0173	-	7470A	PPB	15 Oct 2018 14:02:53	U	SMPL
J5455-06A - 1		13170	3.2928	-	7470A	PPB	15 Oct 2018 14:05:01	U	SMPL
J5455-05LX5 - 1		-25	-0.0073	-	7470A	PPB	15 Oct 2018 14:07:09	U	SMPL
J5455-05A - 1		15963	3.9913	-	7470A	PPB	15 Oct 2018 14:11:46	U	SMPL
CCV87 - 1	CCV87	18228	4.5578	-	7470A	PPB	15 Oct 2018 14:13:53	U	SMPL
CCB87 - 1	CCB87	-102	-0.0265	-	7470A	PPB	15 Oct 2018 14:16:00	U	SMPL