


7471B

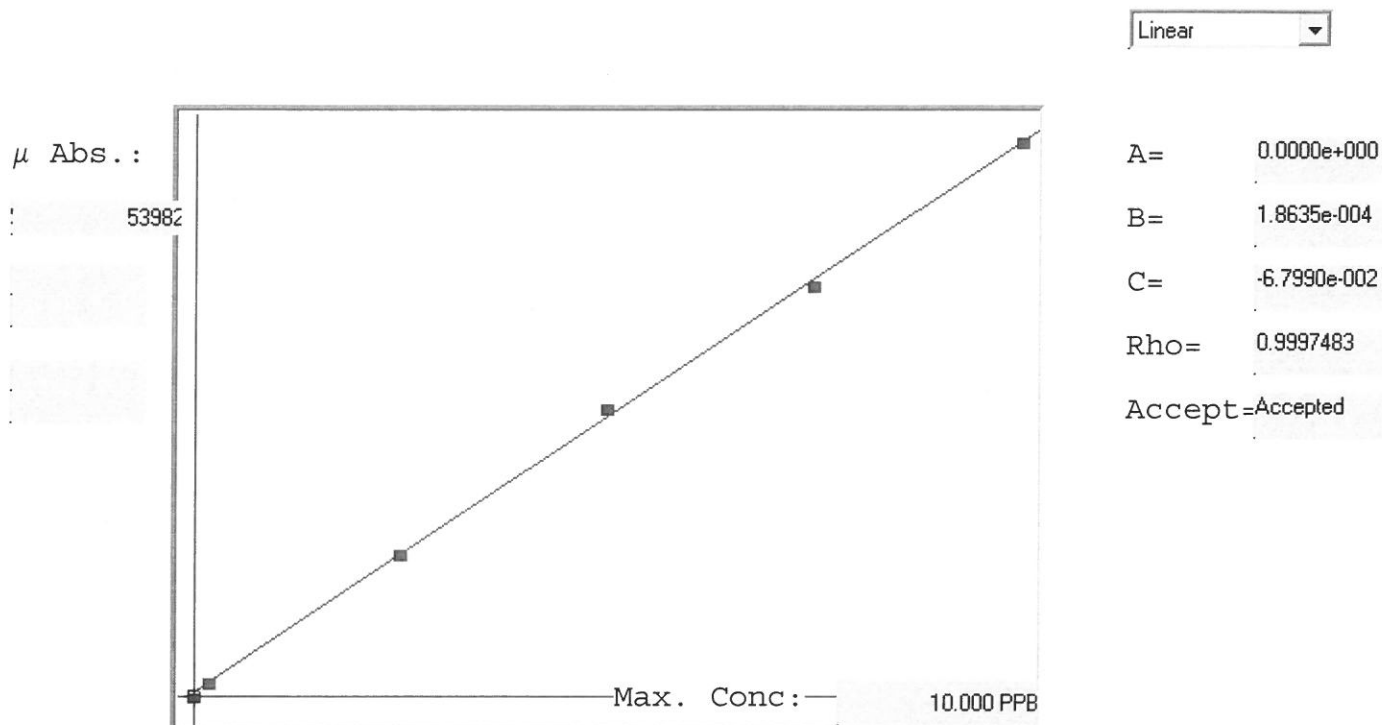

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.067	-0.067	4	0.000	4				
0.2	0.200	0.205	0.005	1465	0.0 %	1465				
2.5	2.500	2.519	0.019	13880	0.0 %	13880				
5.0	5.000	5.158	0.158	28044	0.0 %	28044				
7.5	7.500	7.394	-0.106	40044	0.0 %	40044				
10.0	10.000	9.992	-0.008	53982	0.0 %	53982				

LB98794 INSTRUMENT ID:CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Oct 2018 16:42:14

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	4	-	0.0000	7471B	PPB	23 Oct 2018 17:19:22	S	Std
0.2 - 1	50.2	1465	-	0.2000	7471B	PPB	23 Oct 2018 17:21:40	S	Std
2.5 - 1	52.5	13880	-	2.5000	7471B	PPB	23 Oct 2018 17:23:58	S	Std
5.0 - 1	55.0	28044	-	5.0000	7471B	PPB	23 Oct 2018 17:26:15	S	Std
7.5 - 1	57.5	40044	-	7.5000	7471B	PPB	23 Oct 2018 17:28:33	S	Std
10.0 - 1	59.0	53982	-	10.0000	7471B	PPB	23 Oct 2018 17:30:50	S	Std
ICV34 - 1	ICV34	21676	3.9713	-	7471B	PPB	23 Oct 2018 17:47:24	U	SMPL
ICB34 - 1	ICB34	150	-0.0400	-	7471B	PPB	23 Oct 2018 17:49:40	U	SMPL
CCV58 - 1	CCV58	28108	5.1699	-	7471B	PPB	23 Oct 2018 17:51:56	U	SMPL
CCB58 - 1	CCB58	132	-0.0434	-	7471B	PPB	23 Oct 2018 17:54:12	U	SMPL
CRA - 1	CRA	1523	0.2158	-	7471B	PPB	23 Oct 2018 17:56:28	U	SMPL
HighStd - 1	HighStd	54242	10.0400	-	7471B	PPB	23 Oct 2018 17:58:45	U	SMPL
ChkStd - 1	ChkStd	38225	7.0552	-	7471B	PPB	23 Oct 2018 18:11:44	U	SMPL
PB114043BL - 1	PBS0143	273	-0.0171	-	7471B	PPB	23 Oct 2018 18:14:00	U	SMPL
PB114043BS - 1	LCS0143	19453	3.5571	-	7471B	PPB	23 Oct 2018 18:16:18	U	SMPL
J5197-03 - 1	HD-02-101918	4688	0.8056	-	7471B	PPB	23 Oct 2018 18:18:35	U	SMPL
J5197-03DUP - 1	HD-02-101918DUP	3968	0.6714	-	7471B	PPB	23 Oct 2018 18:20:52	U	SMPL
J5197-03MS - 1	HD-02-101918MS	22323	4.0919	-	7471B	PPB	23 Oct 2018 18:23:09	U	SMPL
J5197-03MSD - 1	HD-02-101918MSD	23257	4.2659	-	7471B	PPB	23 Oct 2018 18:25:28	U	SMPL
J5604-01 - 1	MS-VB-29736-BOX-2	458710	HIGH	-	7471B	PPB	23 Oct 2018 18:27:43	X	
CCV59 - 1	CCV59	27865	5.1246	-	7471B	PPB	23 Oct 2018 18:29:34	U	SMPL
CCB59 - 1	CCB59	25	-0.0633	-	7471B	PPB	23 Oct 2018 18:32:06	U	SMPL
J5604-03 - 1	MS-VB-25868-BOX-1	458526	HIGH	-	7471B	PPB	23 Oct 2018 18:34:22	X	
J5605-01 - 1	TP-A	5326	0.9245	-	7471B	PPB	23 Oct 2018 18:36:14	U	SMPL
J5605-07 - 1	TP-B	3698	0.6211	-	7471B	PPB	23 Oct 2018 18:39:03	U	SMPL
J5606-01 - 1	SOIL-PILE	9878	1.7728	-	7471B	PPB	23 Oct 2018 18:41:20	U	SMPL
J5197-03LX5 - 1		947	0.1085	-	7471B	PPB	23 Oct 2018 18:43:36	U	SMPL
J5197-03A - 1		25623	4.7068	-	7471B	PPB	23 Oct 2018 18:45:53	U	SMPL
J5604-01DLX10 - 1		78208	14.5060	-	7471B	PPB	23 Oct 2018 18:48:10	U	SMPL
J5604-03DLX10 - 1		80932	15.0136	-	7471B	PPB	23 Oct 2018 18:54:04	U	SMPL
J5604-01DL2X50 - 1		16953	3.0912	-	7471B	PPB	23 Oct 2018 18:56:22	U	SMPL
J5604-03DL2X50 - 1		16689	3.0420	-	7471B	PPB	23 Oct 2018 18:58:41	U	SMPL
CCV60 - 1	CCV60	28169	5.1813	-	7471B	PPB	23 Oct 2018 19:00:57	U	SMPL
CCB60 - 1	CCB60	50	-0.0587	-	7471B	PPB	23 Oct 2018 19:03:13	U	SMPL