


LB98818 INSTRUMENT ID: CV1

245.1

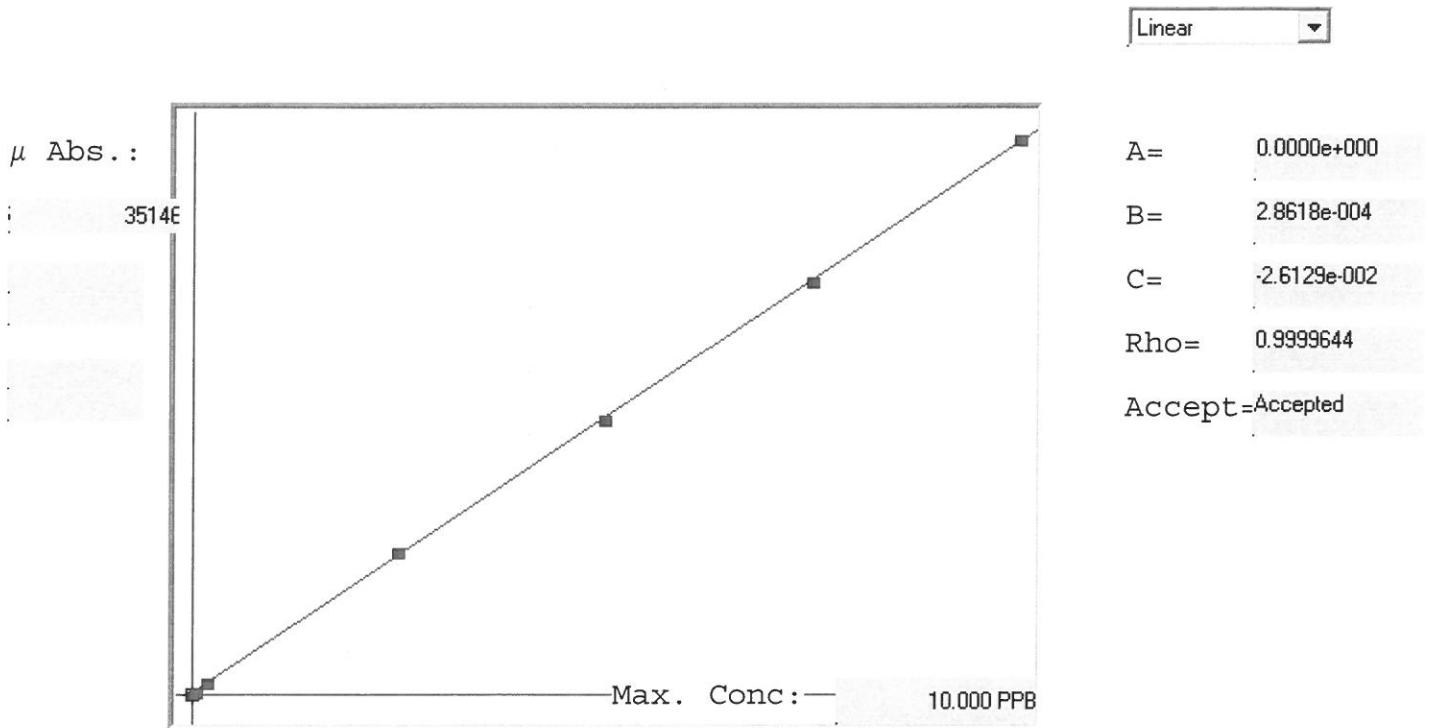

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	71	0.000	71				
0.05	0.050	0.038	-0.012	223	0.0 %	223				
0.2	0.200	0.204	0.004	805	0.0 %	805				
2.5	2.500	2.555	0.055	9018	0.0 %	9018				
5.0	5.000	4.967	-0.033	17448	0.0 %	17448				
7.5	7.500	7.460	-0.040	26160	0.0 %	26160				
10.0	10.000	10.032	0.032	35146	0.0 %	35146				

LB98818 INSTRUMENT ID:CV1

Method: 245.1		Operator: Admin		Date of Analysis: 24 Oct 2018 16:36:50				
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	50.0	71	-	0.0000	245.1	PPB	24 Oct 2018 17:20:04	S Std
0.05 - 1	50.05	223	-	0.0500	245.1	PPB	24 Oct 2018 17:22:22	S Std
0.2 - 1	50.2	805	-	0.2000	245.1	PPB	24 Oct 2018 17:24:39	S Std
2.5 - 1	52.5	9018	-	2.5000	245.1	PPB	24 Oct 2018 17:26:57	S Std
5.0 - 1	55.0	17448	-	5.0000	245.1	PPB	24 Oct 2018 17:29:14	S Std
7.5 - 1	57.5	26160	-	7.5000	245.1	PPB	24 Oct 2018 17:31:31	S Std
10.0 - 1	50.0	35146	-	10.0000	245.1	PPB	24 Oct 2018 17:40:46	S Std
ICV37 - 1	ICV37	15010	4.2694	-245.1		PPB	24 Oct 2018 17:44:15	U SMPL
ICB37 - 1	ICB37	141	0.0142	-245.1		PPB	24 Oct 2018 17:46:30	U SMPL
CCV69 - 1	CCV69	17572	5.0026	-245.1		PPB	24 Oct 2018 17:51:38	U SMPL
CCB69 - 1	CCB69	146	0.0157	-245.1		PPB	24 Oct 2018 17:53:53	U SMPL
CRA - 1	CRA	218	0.0363	-245.1		PPB	24 Oct 2018 17:56:09	U SMPL
HighStd - 1	HighStd	0	-0.0261	-245.1		PPB	24 Oct 2018 17:58:25	U SMPL
HighStd - 1	HighStd	34973	9.9824	-245.1		PPB	24 Oct 2018 18:00:17	U SMPL
ChkStd - 1	ChkStd	25890	7.3830	-245.1		PPB	24 Oct 2018 18:02:32	U SMPL
PB114106BL - 1	PBS0116	-86	-0.0507	-245.1		PPB	24 Oct 2018 18:04:51	U SMPL
PB114106BS - 1	LCS0116	12719	3.6138	-245.1		PPB	24 Oct 2018 18:07:09	U SMPL
J5593-01 - 1	101718-TIPC-E-D-M	-73	-0.0470	-245.1		PPB	24 Oct 2018 18:09:26	U SMPL
J5593-02 - 1	101718-TIPC-E-U-M	-8	-0.0284	-245.1		PPB	24 Oct 2018 18:11:44	U SMPL
J5593-03 - 1	101718-SIDI-E-D-B	18	-0.0210	-245.1		PPB	24 Oct 2018 18:14:01	U SMPL
J5593-04 - 1	101718-SIDI-E-D-M	-3	-0.0270	-245.1		PPB	24 Oct 2018 18:16:19	U SMPL
J5593-05 - 1	101718-SIDI-E-D-S	6	-0.0244	-245.1		PPB	24 Oct 2018 18:18:35	U SMPL
CCV70 - 1	CCV70	17695	5.0378	-245.1		PPB	24 Oct 2018 18:20:51	U SMPL
CCB70 - 1	CCB70	-17	-0.0310	-245.1		PPB	24 Oct 2018 18:23:06	U SMPL
J5593-06 - 1	101718-DBRI-E-D-B	30	-0.0175	-245.1		PPB	24 Oct 2018 18:25:24	U SMPL
J5593-07 - 1	101718-DBRI-E-D-M	5	-0.0247	-245.1		PPB	24 Oct 2018 18:27:40	U SMPL
J5593-08 - 1	101718-DBRI-E-D-S	3	-0.0253	-245.1		PPB	24 Oct 2018 18:29:56	U SMPL
J5593-09 - 1	101718-DBRI-E-U-B	34	-0.0164	-245.1		PPB	24 Oct 2018 18:32:12	U SMPL
J5593-10 - 1	101718-DBRI-E-U-M	0	-0.0261	-245.1		PPB	24 Oct 2018 18:34:29	U SMPL
J5593-11 - 1	101718-DBRI-E-U-S	-2	-0.0267	-245.1		PPB	24 Oct 2018 18:36:46	U SMPL
J5593-12 - 1	101718-JETT-E-D-B	45	-0.0133	-245.1		PPB	24 Oct 2018 18:39:03	U SMPL
J5593-13 - 1	101718-JETT-E-D-M	-3	-0.0270	-245.1		PPB	24 Oct 2018 18:41:20	U SMPL
J5593-14 - 1	101718-JETT-E-D-S	2	-0.0256	-245.1		PPB	24 Oct 2018 18:43:38	U SMPL
J5593-15 - 1	101718-JETT-E-U-B	9	-0.0236	-245.1		PPB	24 Oct 2018 18:45:54	U SMPL
CCV71 - 1	CCV71	17774	5.0604	-245.1		PPB	24 Oct 2018 18:48:10	U SMPL
CCB71 - 1	CCB71	9	-0.0236	-245.1		PPB	24 Oct 2018 18:50:27	U SMPL
J5593-16 - 1	101718-JETT-E-U-M	3	-0.0253	-245.1		PPB	24 Oct 2018 18:52:44	U SMPL
J5593-17 - 1	101718-JETT-E-U-S	19	-0.0207	-245.1		PPB	24 Oct 2018 18:55:00	U SMPL
J5593-17DUP - 1	101718-JETT-E-U-SDUP	-8	-0.0284	-245.1		PPB	24 Oct 2018 18:57:16	U SMPL
J5593-17MS - 1	101718-JETT-E-U-SMS	14189	4.0344	-245.1		PPB	24 Oct 2018 18:59:33	U SMPL
J5593-17MSD - 1	101718-JETT-E-U-SMSD	13704	3.8957	-245.1		PPB	24 Oct 2018 19:01:49	U SMPL
J5593-17LX5 - 1		133	0.0119	-245.1		PPB	24 Oct 2018 19:04:06	U SMPL
J5593-17A - 1		16210	4.6128	-245.1		PPB	24 Oct 2018 19:06:23	U SMPL
PB114031BL - 1	PBS0131	30	-0.0175	-245.1		PPB	24 Oct 2018 19:08:41	U SMPL
PB114031BS - 1	LCS0131	14220	4.0433	-245.1		PPB	24 Oct 2018 19:10:58	U SMPL
J5601-01 - 1	101818-SIDI-E-D-B	-13	-0.0298	-245.1		PPB	24 Oct 2018 19:13:15	U SMPL
CCV72 - 1	CCV72	17809	5.0704	-245.1		PPB	24 Oct 2018 19:15:31	U SMPL
CCB72 - 1	CCB72	122	0.0088	-245.1		PPB	24 Oct 2018 19:17:47	U SMPL
J5601-02 - 1	101818-SIDE-E-D-M	-16	-0.0307	-245.1		PPB	24 Oct 2018 19:20:04	U SMPL
J5601-03 - 1	101818-SIDE-E-D-S	0	-0.0261	-245.1		PPB	24 Oct 2018 19:22:20	U SMPL
J5601-04 - 1	101818-SIDE-E-U-B	51	-0.0115	-245.1		PPB	24 Oct 2018 19:24:37	U SMPL
J5601-05 - 1	101818-SIDE-E-U-M	12	-0.0227	-245.1		PPB	24 Oct 2018 19:26:53	U SMPL
J5601-06 - 1	101818-SIDE-E-U-S	19	-0.0207	-245.1		PPB	24 Oct 2018 19:29:10	U SMPL
J5601-07 - 1	101818-TIPC-E-D-M	13	-0.0224	-245.1		PPB	24 Oct 2018 19:31:27	U SMPL
J5601-08 - 1	101818-TIPC-E-U-M	1	-0.0258	-245.1		PPB	24 Oct 2018 19:33:44	U SMPL
J5601-08DUP - 1	101818-TIPC-E-U-M	30	-0.0175	-245.1		PPB	24 Oct 2018 19:36:02	U SMPL
J5601-08MS - 1	101818-TIPC-E-U-M	14422	4.1011	-245.1		PPB	24 Oct 2018 19:38:20	U SMPL
J5601-08MSD - 1	101818-TIPC-E-U-M	14336	4.0765	-245.1		PPB	24 Oct 2018 19:40:37	U SMPL
CCV73 - 1	CCV73	18153	5.1689	-245.1		PPB	24 Oct 2018 19:42:53	U SMPL
CCB73 - 1	CCB73	47	-0.0127	-245.1		PPB	24 Oct 2018 19:45:09	U SMPL
J5601-08LX5 - 1		57	-0.0098	-245.1		PPB	24 Oct 2018 19:47:26	U SMPL
J5601-08A - 1		16830	4.7902	-245.1		PPB	24 Oct 2018 19:49:43	U SMPL
CCV74 - 1	CCV74	17673	5.0315	-245.1		PPB	24 Oct 2018 19:51:59	U SMPL
CCB74 - 1	CCB74	7	-0.0241	-245.1		PPB	24 Oct 2018 19:54:16	U SMPL