

LB98916 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 30 Oct 2018 08:37:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	104	-	0.0000	7471B	PPB	30 Oct 2018 08:51:26	S	Std
0.2 - 1	50'2	1169	-	0.2000	7471B	PPB	30 Oct 2018 08:53:44	S	Std
2.5 - 1	52.5	12490	-	2.5000	7471B	PPB	30 Oct 2018 08:56:02	S	Std
5.0 - 1	55	25171	-	5.0000	7471B	PPB	30 Oct 2018 08:58:20	S	Std
7.5 - 1	57.5	37001	-	7.5000	7471B	PPB	30 Oct 2018 09:00:37	S	Std
10.0 - 1	510	49934	-	10.0000	7471B	PPB	30 Oct 2018 09:02:55	S	Std
ICV46 - 1	ICV46	19769	3.9564	-	7471B	PPB	30 Oct 2018 09:05:46	U	SMPL
ICB46 - 1	ICB46	-8	-0.0277	-	7471B	PPB	30 Oct 2018 09:08:01	U	SMPL
CCV14 - 1	CCV14	25046	5.0195	-	7471B	PPB	30 Oct 2018 09:10:18	U	SMPL
CCB14 - 1	CCB14	-25	-0.0311	-	7471B	PPB	30 Oct 2018 09:12:33	U	SMPL
CRA - 1	CRA	1154	0.2064	-	7471B	PPB	30 Oct 2018 09:14:50	U	SMPL
HighStd - 1	HighStd	50840	10.2158	-	7471B	PPB	30 Oct 2018 09:17:06	U	SMPL
ChkStd - 1	ChkStd	35014	7.0276	-	7471B	PPB	30 Oct 2018 09:19:22	U	SMPL
PB114292BL - 1	PBS	-17	-0.0295	-	7471B	PPB	30 Oct 2018 09:21:41	U	SMPL
PB114292BS - 1	LCSS	18507	3.7022	-	7471B	PPB	30 Oct 2018 09:23:59	U	SMPL
J5194-07 - 1	HR-05-102618-A	3678	0.7148	-	7471B	PPB	30 Oct 2018 09:26:16	U	SMPL
J5194-09 - 1	HR-05-102618-B	47667	9.5765	-	7471B	PPB	30 Oct 2018 09:28:33	U	SMPL
J5194-11 - 1	HR-05-102618-C	31326	6.2846	-	7471B	PPB	30 Oct 2018 09:30:51	U	SMPL
J5204-09 - 1	SU-02-102518-A	2092	0.3953	-	7471B	PPB	30 Oct 2018 09:33:10	U	SMPL
J5204-11 - 1	SU-02-102518-B	2537	0.4850	-	7471B	PPB	30 Oct 2018 09:35:27	U	SMPL
CCV15 - 1	CCV15	25215	5.0535	-	7471B	PPB	30 Oct 2018 09:37:43	U	SMPL
CCB15 - 1	CCB15	15	-0.0231	-	7471B	PPB	30 Oct 2018 09:39:59	U	SMPL
J5204-13 - 1	SU-01-102518-A	2786	0.5351	-	7471B	PPB	30 Oct 2018 09:42:16	U	SMPL
J5204-15 - 1	SU-01-102518-B	2172	0.4114	-	7471B	PPB	30 Oct 2018 09:44:31	U	SMPL
J5205-05 - 1	TR-05-102518	1656	0.3075	-	7471B	PPB	30 Oct 2018 09:46:48	U	SMPL
J5649-01 - 1	DL-01A	2753	0.5285	-	7471B	PPB	30 Oct 2018 09:49:04	U	SMPL
J5649-02 - 1	DL-01B	2393	0.4560	-	7471B	PPB	30 Oct 2018 09:51:21	U	SMPL
J5649-03 - 1	DL-02A	1276	0.2309	-	7471B	PPB	30 Oct 2018 09:53:38	U	SMPL
J5649-04 - 1	DL-02B	790	0.1330	-	7471B	PPB	30 Oct 2018 09:55:55	U	SMPL
J5649-05 - 1	DL-02C	911	0.1574	-	7471B	PPB	30 Oct 2018 09:58:13	U	SMPL
J5649-06 - 1	DL-03A	5899	1.1623	-	7471B	PPB	30 Oct 2018 10:00:30	U	SMPL
J5649-06DUP - 1	DL-03ADUP	5598	1.1016	-	7471B	PPB	30 Oct 2018 10:02:47	U	SMPL
CCV16 - 1	CCV16	25404	5.0916	-	7471B	PPB	30 Oct 2018 10:05:04	U	SMPL
CCB16 - 1	CCB16	-5	-0.0271	-	7471B	PPB	30 Oct 2018 10:07:21	U	SMPL
J5649-07 - 1	J5649-06MS	25915	5.1945	-	7471B	PPB	30 Oct 2018 10:09:38	U	SMPL
J5649-08 - 1	J5649-06MSD	25377	5.0862	-	7471B	PPB	30 Oct 2018 10:11:55	U	SMPL
J5649-09 - 1	DL-03B	208	0.0158	-	7471B	PPB	30 Oct 2018 10:14:12	U	SMPL
J5649-10 - 1	DL-04A	1746	0.3256	-	7471B	PPB	30 Oct 2018 10:16:29	U	SMPL
J5649-11 - 1	DL-04B	164	0.0069	-	7471B	PPB	30 Oct 2018 10:18:46	U	SMPL
J5649-12 - 1	DL-05A	911	0.1574	-	7471B	PPB	30 Oct 2018 10:21:03	U	SMPL
J5649-13 - 1	DL-05B	160	0.0061	-	7471B	PPB	30 Oct 2018 10:23:20	U	SMPL
PB114293BL - 1	PBS	130	0.0001	-	7471B	PPB	30 Oct 2018 10:25:37	U	SMPL
PB114293BS - 1	LCSS	20363	4.0761	-	7471B	PPB	30 Oct 2018 10:27:54	U	SMPL
J5675-01 - 1	TP-5	9091	1.8053	-	7471B	PPB	30 Oct 2018 10:30:11	U	SMPL
CCV17 - 1	CCV17	25611	5.1333	-	7471B	PPB	30 Oct 2018 10:32:28	U	SMPL
CCB17 - 1	CCB17	2	-0.0257	-	7471B	PPB	30 Oct 2018 10:34:45	U	SMPL
J5675-05 - 1	TP-13	11525	2.2956	-	7471B	PPB	30 Oct 2018 10:37:02	U	SMPL
J5683-01 - 1	SP-SAMPLE	1628	0.3019	-	7471B	PPB	30 Oct 2018 10:39:19	U	SMPL
J5685-01 - 1	DOCUMENTATION-25	10601	2.1095	-	7471B	PPB	30 Oct 2018 10:41:36	U	SMPL
J5685-02 - 1	DOCUMENTATION-26	6088	1.2003	-	7471B	PPB	30 Oct 2018 10:43:53	U	SMPL
J5685-03 - 1	DOCUMENTATION-27	19600	3.9224	-	7471B	PPB	30 Oct 2018 10:46:10	U	SMPL
J5685-04 - 1	DOCUMENTATION-28	18908	3.7830	-	7471B	PPB	30 Oct 2018 10:48:27	U	SMPL
J5685-05 - 1	DOCUMENTATION-29	15916	3.1802	-	7471B	PPB	30 Oct 2018 10:50:44	U	SMPL
J5685-06 - 1	DOCUMENTATION-30	9642	1.9163	-	7471B	PPB	30 Oct 2018 10:53:01	U	SMPL
J5685-07 - 1	DOCUMENTATION-31	10211	2.0309	-	7471B	PPB	30 Oct 2018 10:55:18	U	SMPL
J5685-08 - 1	DOCUMENTATION-32	15264	3.0489	-	7471B	PPB	30 Oct 2018 10:57:35	U	SMPL
CCV18 - 1	CCV18	25826	5.1766	-	7471B	PPB	30 Oct 2018 11:00:00	U	SMPL
CCB18 - 1	CCB18	3	-0.0255	-	7471B	PPB	30 Oct 2018 11:02:17	U	SMPL
J5688-01 - 1	DPC-91567-OD-01	188	0.0118	-	7471B	PPB	30 Oct 2018 11:04:34	U	SMPL
J5696-01 - 1	DL-SED-01	31409	6.3013	-	7471B	PPB	30 Oct 2018 11:06:51	U	SMPL
J5696-01DUP - 1	DL-SED-01DUP	32306	6.4820	-	7471B	PPB	30 Oct 2018 11:09:08	U	SMPL
J5696-03 - 1	J5696-01MSD	47822	9.6078	-	7471B	PPB	30 Oct 2018 11:11:25	U	SMPL
J5696-02 - 1	J5696-01MS	49549	9.9557	-	7471B	PPB	30 Oct 2018 11:13:42	U	SMPL
J5696-04 - 1	DL-SED-02	34130	6.8495	-	7471B	PPB	30 Oct 2018 11:15:59	U	SMPL
J5697-01 - 1	CHRT-58-66-98-92	2583	0.4942	-	7471B	PPB	30 Oct 2018 11:18:16	U	SMPL
CCV19 - 1	CCV19	25869	5.1853	-	7471B	PPB	30 Oct 2018 11:20:33	U	SMPL
CCB19 - 1	CCB19	-9	-0.0279	-	7471B	PPB	30 Oct 2018 11:22:50	U	SMPL
J5649-06LX5 - 1		1154	0.2064	-	7471B	PPB	30 Oct 2018 11:25:07	U	SMPL
J5649-06A - 1		25827	5.1768	-	7471B	PPB	30 Oct 2018 11:27:24	U	SMPL
J5696-01LX5 - 1		6220	1.2269	-	7471B	PPB	30 Oct 2018 11:29:41	U	SMPL
J5696-01A - 1		48630	9.7705	-	7471B	PPB	30 Oct 2018 11:31:58	U	SMPL
CCV20 - 1	CCV20	25531	5.1172	-	7471B	PPB	30 Oct 2018 11:34:15	U	SMPL
CCB20 - 1	CCB20	-14	-0.0289	-	7471B	PPB	30 Oct 2018 11:36:32	U	SMPL

L13 9 8 916


7471B

INSTRUMENT ID: CV1

Linear

μ Abs.:

49934

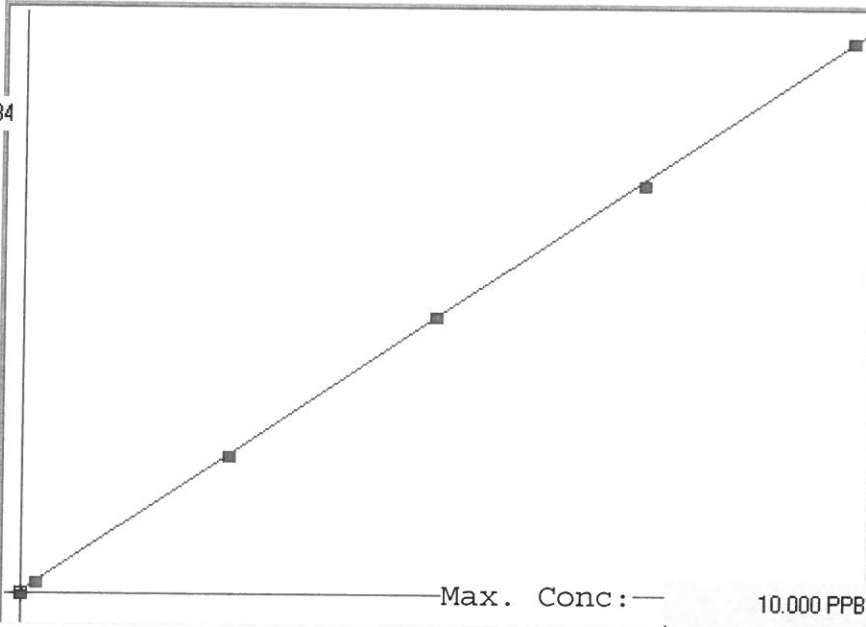

A= 0.0000e+000

B= 2.0145e-004

C= -2.6113e-002

Rho= 0.9999479

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.005	-0.005	104	0.000	104				
0.2	0.200	0.209	0.009	1169	0.0 %	1169				
2.5	2.500	2.490	-0.010	12490	0.0 %	12490				
5.0	5.000	5.045	0.045	25171	0.0 %	25171				
7.5	7.500	7.428	-0.072	37001	0.0 %	37001				
10.0	10.000	10.033	0.033	49934	0.0 %	49934				