

LB 98940


7470A

INSTRUMENT ID : CV1

Linear

 μ Abs.:

34245

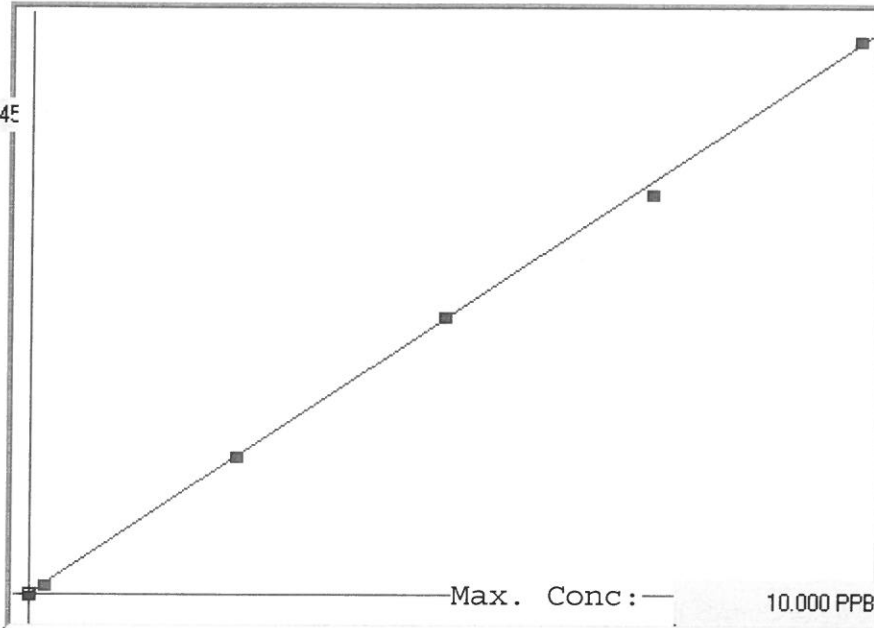

A= 0.0000e+000

B= 2.9468e-004

C= -1.1485e-002

Rho= 0.9997136

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.009	-0.009	9	0.000	9				
0.2	0.200	0.191	-0.009	687	0.0 %	687				
2.5	2.500	2.534	0.034	8638	0.0 %	8638				
5.0	5.000	5.083	0.083	17290	0.0 %	17290				
7.5	7.500	7.321	-0.179	24882	0.0 %	24882				
10.0	10.000	10.080	0.080	34245	0.0 %	34245				

LB98940 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Oct 2018 09:15:49

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	9	-	0.0000	7470A	PPB	31 Oct 2018 09:20:23	S	Std
0.2 - 1	50.2	687	-	0.2000	7470A	PPB	31 Oct 2018 09:22:32	S	Std
2.5 - 1	52.5	8638	-	2.5000	7470A	PPB	31 Oct 2018 09:24:41	S	Std
5.0 - 1	55	17290	-	5.0000	7470A	PPB	31 Oct 2018 09:26:50	S	Std
7.5 - 1	57.5	24882	-	7.5000	7470A	PPB	31 Oct 2018 09:28:57	S	Std
10.0 - 1	510	34245	-	10.0000	7470A	PPB	31 Oct 2018 09:31:05	S	Std
ICV48 - 1	ICV48	14148	4.1576	-7470A	PPB	PPB	31 Oct 2018 09:33:38	U	SMPL
ICB48 - 1	ICB48	-118	-0.0463	-7470A	PPB	PPB	31 Oct 2018 09:35:45	U	SMPL
CCV33 - 1	CCV33	17226	5.0646	-7470A	PPB	PPB	31 Oct 2018 09:37:51	U	SMPL
CCB33 - 1	CCB33	-107	-0.0430	-7470A	PPB	PPB	31 Oct 2018 09:39:58	U	SMPL
CRA - 1	CRA	673	0.1868	-7470A	PPB	PPB	31 Oct 2018 09:42:04	U	SMPL
HighStd - 1	HighStd	34158	10.0541	-7470A	PPB	PPB	31 Oct 2018 09:44:11	U	SMPL
ChkStd - 1	ChkStd	24179	7.1135	-7470A	PPB	PPB	31 Oct 2018 09:46:19	U	SMPL
PB114279BL - 1	PBW	-34	-0.0215	-7470A	PPB	PPB	31 Oct 2018 09:50:54	U	SMPL
PB114279BS - 1	LCSW	15066	4.4281	-7470A	PPB	PPB	31 Oct 2018 09:53:01	U	SMPL
J5194-10 - 1	HR-05-102618-B	802	0.2248	-7470A	PPB	PPB	31 Oct 2018 10:08:47	U	SMPL
CCV34 - 1	CCV34	17291	5.0838	-7470A	PPB	PPB	31 Oct 2018 10:10:54	U	SMPL
CCB34 - 1	CCB34	-96	-0.0398	-7470A	PPB	PPB	31 Oct 2018 10:13:01	U	SMPL
J5194-12 - 1	HR-05-102618-C	824	0.2313	-7470A	PPB	PPB	31 Oct 2018 10:15:08	U	SMPL
J5697-02 - 1	CHRT-58-66-98-92	1058	0.3003	-7470A	PPB	PPB	31 Oct 2018 10:17:14	U	SMPL
PB114280BS - 1	LCSW	14073	4.1355	-7470A	PPB	PPB	31 Oct 2018 10:21:28	U	SMPL
J5627-02 - 1	BP-LF1-SPW-1D-10-18	-109	-0.0436	-7470A	PPB	PPB	31 Oct 2018 10:23:35	U	SMPL
J5627-04 - 1	BP-LF1-SPW-2D-10-18	-68	-0.0315	-7470A	PPB	PPB	31 Oct 2018 10:25:43	U	SMPL
J5627-05 - 1	BP-LF1-SPW-EB-10-18	-76	-0.0339	-7470A	PPB	PPB	31 Oct 2018 10:27:51	U	SMPL
J5690-01 - 1	MW-15	986	0.2791	-7470A	PPB	PPB	31 Oct 2018 10:29:59	U	SMPL
J5690-01DUP - 1	MW-15DUP	873	0.2458	-7470A	PPB	PPB	31 Oct 2018 10:32:07	U	SMPL
J5690-02 - 1	J5690-01MS	15335	4.5074	-7470A	PPB	PPB	31 Oct 2018 10:34:14	U	SMPL
CCV35 - 1	CCV35	17095	5.0260	-7470A	PPB	PPB	31 Oct 2018 10:36:21	U	SMPL
CCB35 - 1	CCB35	-115	-0.0454	-7470A	PPB	PPB	31 Oct 2018 10:38:28	U	SMPL
J5690-03 - 1	J5690-01MSD	14666	4.3103	-7470A	PPB	PPB	31 Oct 2018 10:40:36	U	SMPL
J5690-04 - 1	MW-202	871	0.2452	-7470A	PPB	PPB	31 Oct 2018 10:42:43	U	SMPL
J5692-20 - 1	CAL-IDW-20181025	824	0.2313	-7470A	PPB	PPB	31 Oct 2018 10:44:50	U	SMPL
J5696-05 - 1	DL-SW-01	746	0.2083	-7470A	PPB	PPB	31 Oct 2018 10:46:57	U	SMPL
J5696-06 - 1	J5696-05MS	13864	4.0739	-7470A	PPB	PPB	31 Oct 2018 10:52:41	U	SMPL
J5696-07 - 1	J5696-05MSD	13960	4.1022	-7470A	PPB	PPB	31 Oct 2018 10:54:48	U	SMPL
J5696-08 - 1	DL-SW-02	1533	0.4403	-7470A	PPB	PPB	31 Oct 2018 10:56:56	U	SMPL
J5696-09 - 1	EB-2018.10.25-GW	5445	1.5930	-7470A	PPB	PPB	31 Oct 2018 10:59:04	U	SMPL
J5696-10 - 1	EB-2018.10.25-SED	4910	1.4354	-7470A	PPB	PPB	31 Oct 2018 11:01:13	U	SMPL
J5696-11 - 1	EB-2018.10.25-SW	4870	1.4236	-7470A	PPB	PPB	31 Oct 2018 11:03:20	U	SMPL
CCV36 - 1	CCV36	16990	4.9951	-7470A	PPB	PPB	31 Oct 2018 11:05:27	U	SMPL
CCB36 - 1	CCB36	-91	-0.0383	-7470A	PPB	PPB	31 Oct 2018 11:07:34	U	SMPL
J5718-01 - 1	WS-CFA-111C	13	-0.0077	-7470A	PPB	PPB	31 Oct 2018 11:09:42	U	SMPL
PB114329BL - 1	PBW	-23	-0.0183	-7470A	PPB	PPB	31 Oct 2018 11:11:50	U	SMPL
PB114329BS - 1	LCSW	13256	3.8948	-7470A	PPB	PPB	31 Oct 2018 11:13:58	U	SMPL
J5718-02 - 1	WS-CFA-111C	-69	-0.0318	-7470A	PPB	PPB	31 Oct 2018 11:16:05	U	SMPL
J5718-02DUP - 1	WS-CFA-111CDUP	-12	-0.0150	-7470A	PPB	PPB	31 Oct 2018 11:18:12	U	SMPL
J5718-02MS - 1	WS-CFA-111CMS	13704	4.0268	-7470A	PPB	PPB	31 Oct 2018 11:20:20	U	SMPL
J5718-02MSD - 1	WS-CFA-111CMSD	12620	3.7073	-7470A	PPB	PPB	31 Oct 2018 11:22:28	U	SMPL
PB114330BL - 1	PBW	-74	-0.0333	-7470A	PPB	PPB	31 Oct 2018 11:24:36	U	SMPL
PB114330BS - 1	LCSW	13835	4.0654	-7470A	PPB	PPB	31 Oct 2018 11:26:44	U	SMPL
J5719-01 - 1	S1	-57	-0.0283	-7470A	PPB	PPB	31 Oct 2018 11:28:52	U	SMPL
CCV37 - 1	CCV37	17466	5.1354	-7470A	PPB	PPB	31 Oct 2018 11:30:59	U	SMPL
CCB37 - 1	CCB37	-108	-0.0433	-7470A	PPB	PPB	31 Oct 2018 11:33:06	U	SMPL
J5719-01DUP - 1	S1DUP	-15	-0.0159	-7470A	PPB	PPB	31 Oct 2018 11:35:13	U	SMPL
J5719-01MS - 1	S1MS	12302	3.6136	-7470A	PPB	PPB	31 Oct 2018 11:37:20	U	SMPL
J5719-01MSD - 1	S1MSD	13239	3.8898	-7470A	PPB	PPB	31 Oct 2018 11:39:27	U	SMPL
J5719-02 - 1	S2	-62	-0.0298	-7470A	PPB	PPB	31 Oct 2018 11:41:35	U	SMPL
PB114280BL - 1	PBW	-25	-0.0189	-7470A	PPB	PPB	31 Oct 2018 11:43:42	U	SMPL
PB114279TB - 1	PB114241TB	50	0.0032	-7470A	PPB	PPB	31 Oct 2018 11:45:50	U	SMPL
PB114329TB - 1	PB114285TB	20	-0.0056	-7470A	PPB	PPB	31 Oct 2018 11:47:58	U	SMPL
PB114330TB - 1	PB114286TB	29	-0.0029	-7470A	PPB	PPB	31 Oct 2018 11:50:06	U	SMPL
J5194-08 - 1	HR-05-102618-A	25	-0.0041	-7470A	PPB	PPB	31 Oct 2018 11:52:15	U	SMPL
J5194-08DUP - 1	HR-05-102618-ADUP	49	0.0030	-7470A	PPB	PPB	31 Oct 2018 11:54:23	U	SMPL
CCV38 - 1	CCV38	17060	5.0157	-7470A	PPB	PPB	31 Oct 2018 11:56:31	U	SMPL
CCB38 - 1	CCB38	-90	-0.0380	-7470A	PPB	PPB	31 Oct 2018 11:58:38	U	SMPL
J5194-08MS - 1	HR-05-102618-AMS	11483	3.3723	-7470A	PPB	PPB	31 Oct 2018 12:00:46	U	SMPL
J5194-08MSD - 1	HR-05-102618-AMSD	11538	3.3885	-7470A	PPB	PPB	31 Oct 2018 12:02:53	U	SMPL
J5194-08LX5 - 1		-99	-0.0407	-7470A	PPB	PPB	31 Oct 2018 12:05:01	U	SMPL
J5194-08A - 1		12737	3.7418	-7470A	PPB	PPB	31 Oct 2018 12:07:09	U	SMPL
J5690-01LX5 - 1		68	0.0086	-7470A	PPB	PPB	31 Oct 2018 12:09:16	U	SMPL
J5690-01A - 1		15398	4.5260	-7470A	PPB	PPB	31 Oct 2018 12:11:23	U	SMPL
J5718-02LX5 - 1		-90	-0.0380	-7470A	PPB	PPB	31 Oct 2018 12:13:31	U	SMPL
J5718-02A - 1		12859	3.7778	-7470A	PPB	PPB	31 Oct 2018 12:15:40	U	SMPL
J5719-01LX5 - 1		-73	-0.0330	-7470A	PPB	PPB	31 Oct 2018 12:17:49	U	SMPL
J5719-01A - 1		13310	3.9107	-7470A	PPB	PPB	31 Oct 2018 12:19:57	U	SMPL
CCV39 - 1	CCV39	17383	5.1109	-7470A	PPB	PPB	31 Oct 2018 12:22:04	U	SMPL
CCB39 - 1	CCB39	-93	-0.0389	-7470A	PPB	PPB	31 Oct 2018 12:24:12	U	SMPL