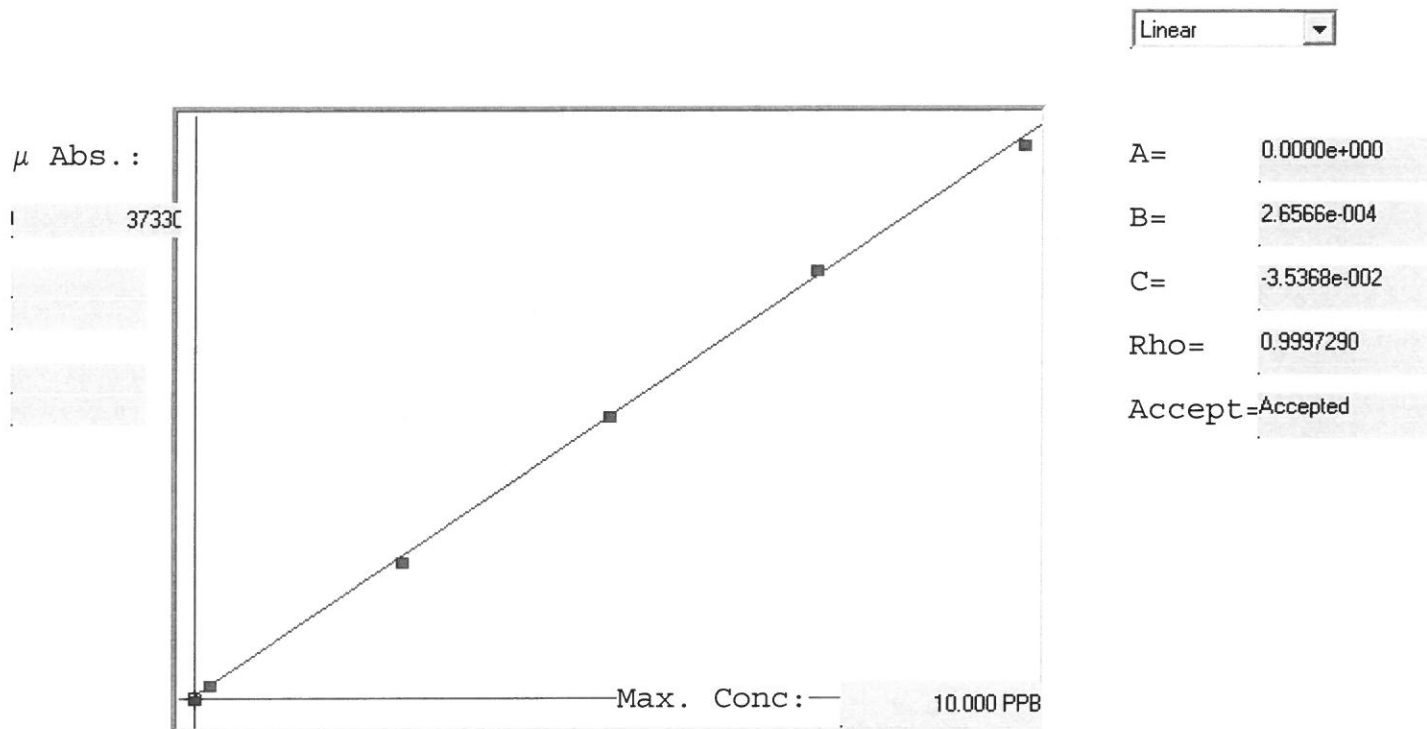


7470A

LB99049
INSTRUMENT ID: CV1

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.041	-0.041	-23	0.000	-23				
0.2	0.200	0.239	0.039	1033	0.0 %	1033				
2.5	2.500	2.437	-0.063	9305	0.0 %	9305				
5.0	5.000	5.037	0.037	19092	0.0 %	19092				
7.5	7.500	7.647	0.147	28919	0.0 %	28919				
10.0	10.000	9.882	-0.118	37330	0.0 %	37330				

LB99049 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Nov 2018 09:21:05

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-23	-	0.0000	7470A	PPB	06 Nov 2018 09:28:42	S	Std
0.2 - 1	502	1033	-	0.2000	7470A	PPB	06 Nov 2018 09:30:51	S	Std
2.5 - 1	52-5	9305	-	2.5000	7470A	PPB	06 Nov 2018 09:35:02	S	Std
5.0 - 1	55	19092	-	5.0000	7470A	PPB	06 Nov 2018 09:37:10	S	Std
7.5 - 1	57-5	28919	-	7.5000	7470A	PPB	06 Nov 2018 09:39:18	S	Std
10.0 - 1	510	37330	-	10.0000	7470A	PPB	06 Nov 2018 09:41:26	S	Std
ICV59 - 1	ICV59	14481	3.8117	-	7470A	PPB	06 Nov 2018 09:44:17	U	SMPL
ICB59 - 1	ICB59	34	-0.0263	-	7470A	PPB	06 Nov 2018 09:48:52	U	SMPL
CCV01 - 1	CCV01	19323	5.0980	-	7470A	PPB	06 Nov 2018 09:53:20	U	SMPL
CCB01 - 1	CCB01	-22	-0.0412	-	7470A	PPB	06 Nov 2018 09:55:26	U	SMPL
CRA - 1	CRA	1030	0.2383	-	7470A	PPB	06 Nov 2018 09:57:33	U	SMPL
HighStd - 1	HighStd	38237	10.1228	-	7470A	PPB	06 Nov 2018 09:59:40	U	SMPL
ChkStd - 1	ChkStd	27058	7.1529	-	7470A	PPB	06 Nov 2018 10:01:46	U	SMPL
PB114503BL - 1	PBW	-178	-0.0827	-	7470A	PPB	06 Nov 2018 10:03:55	U	SMPL
PB114503BS - 1	LCSW	14041	3.6948	-	7470A	PPB	06 Nov 2018 10:06:04	U	SMPL
J5764-02 - 1	JC-03-110218-A	-99	-0.0617	-	7470A	PPB	06 Nov 2018 10:08:11	U	SMPL
J5764-02DUP - 1	JC-03-110218-ADUP	160	0.0071	-	7470A	PPB	06 Nov 2018 10:10:19	U	SMPL
J5764-02MS - 1	JC-03-110218-AMS	13693	3.6023	-	7470A	PPB	06 Nov 2018 10:12:28	U	SMPL
J5764-02MSD - 1	JC-03-110218-AMSD	13947	3.6698	-	7470A	PPB	06 Nov 2018 10:14:37	U	SMPL
J5764-04 - 1	JC-03-110218-B	-109	-0.0643	-	7470A	PPB	06 Nov 2018 10:16:43	U	SMPL
CCV02 - 1	CCV02	19908	5.2534	-	7470A	PPB	06 Nov 2018 10:18:50	U	SMPL
CCB02 - 1	CCB02	-55	-0.0500	-	7470A	PPB	06 Nov 2018 10:42:35	U	SMPL
J5764-06 - 1	JC-03-110218-C	-6	-0.0370	-	7470A	PPB	06 Nov 2018 10:44:41	U	SMPL
J5764-08 - 1	JC-03-110218-D	-7	-0.0372	-	7470A	PPB	06 Nov 2018 10:46:48	U	SMPL
J5764-10 - 1	JC-03-110218-E	-20	-0.0407	-	7470A	PPB	06 Nov 2018 10:48:54	U	SMPL
J5764-12 - 1	JC-03-110218-F	-22	-0.0412	-	7470A	PPB	06 Nov 2018 10:51:02	U	SMPL
J5764-14 - 1	JC-03-110218-G	-31	-0.0436	-	7470A	PPB	06 Nov 2018 10:53:09	U	SMPL
J5764-16 - 1	JC-03-110218-H	-19	-0.0404	-	7470A	PPB	06 Nov 2018 10:55:17	U	SMPL
J5764-18 - 1	JC-03-110218-I	-14	-0.0391	-	7470A	PPB	06 Nov 2018 10:57:25	U	SMPL
J5764-20 - 1	JC-03-110218-J	-20	-0.0407	-	7470A	PPB	06 Nov 2018 10:59:33	U	SMPL
J5805-01 - 1	COMP-SAMPLES(1-5)	-13	-0.0388	-	7470A	PPB	06 Nov 2018 11:01:42	U	SMPL
J5805-02 - 1	COMP-SAMPLES(6-10)	-9	-0.0378	-	7470A	PPB	06 Nov 2018 11:03:49	U	SMPL
CCV03 - 1	CCV03	19678	5.1923	-	7470A	PPB	06 Nov 2018 11:05:56	U	SMPL
CCB03 - 1	CCB03	-93	-0.0601	-	7470A	PPB	06 Nov 2018 11:08:02	U	SMPL
J5805-03 - 1	COMP-SAMPLES(11-15)	-43	-0.0468	-	7470A	PPB	06 Nov 2018 11:10:10	U	SMPL
J5805-04 - 1	COMP-SAMPLES(16-20)	-32	-0.0439	-	7470A	PPB	06 Nov 2018 11:12:16	U	SMPL
J5805-05 - 1	COMP-SAMPLES(21-25)	-21	-0.0409	-	7470A	PPB	06 Nov 2018 11:14:23	U	SMPL
J5805-06 - 1	COMP-SAMPLES(26-30)	-4	-0.0364	-	7470A	PPB	06 Nov 2018 11:16:31	U	SMPL
J5805-07 - 1	COMP-SAMPLES(31-35)	-26	-0.0423	-	7470A	PPB	06 Nov 2018 11:18:38	U	SMPL
J5805-08 - 1	COMP-SAMPLES(36-40)	10	-0.0327	-	7470A	PPB	06 Nov 2018 11:20:46	U	SMPL
J5805-09 - 1	COMP-SAMPLES(41-45)	-10	-0.0380	-	7470A	PPB	06 Nov 2018 11:22:54	U	SMPL
PB114506BL - 1	PBW	22	-0.0295	-	7470A	PPB	06 Nov 2018 11:25:02	U	SMPL
PB114506BS - 1	LCSW	14263	3.7538	-	7470A	PPB	06 Nov 2018 11:27:11	U	SMPL
J5735-23 - 1	12B	-103	-0.0627	-	7470A	PPB	06 Nov 2018 11:29:18	U	SMPL
CCV04 - 1	CCV04	19648	5.1844	-	7470A	PPB	06 Nov 2018 11:31:25	U	SMPL
CCB04 - 1	CCB04	-34	-0.0444	-	7470A	PPB	06 Nov 2018 11:33:32	U	SMPL
J5745-21 - 1	12H	-16	-0.0396	-	7470A	PPB	06 Nov 2018 11:35:40	U	SMPL
J5745-22 - 1	6A	-8	-0.0375	-	7470A	PPB	06 Nov 2018 11:37:47	U	SMPL
J5745-23 - 1	6B	-27	-0.0425	-	7470A	PPB	06 Nov 2018 11:39:54	U	SMPL
J5745-25 - 1	8A	33	-0.0266	-	7470A	PPB	06 Nov 2018 11:42:01	U	SMPL
J5745-26 - 1	8B	-7	-0.0372	-	7470A	PPB	06 Nov 2018 11:44:09	U	SMPL
J5750-10 - 1	7A	8	-0.0332	-	7470A	PPB	06 Nov 2018 11:46:16	U	SMPL
J5750-11 - 1	7B	-7	-0.0372	-	7470A	PPB	06 Nov 2018 11:48:24	U	SMPL
J5750-12 - 1	7C	-29	-0.0431	-	7470A	PPB	06 Nov 2018 11:50:33	U	SMPL
J5771-02 - 1	EO-01-110218-A	7	-0.0335	-	7470A	PPB	06 Nov 2018 11:52:41	U	SMPL
J5771-02DUP - 1	EO-01-110218-ADUP	-31	-0.0436	-	7470A	PPB	06 Nov 2018 11:54:49	U	SMPL
CCV05 - 1	CCV05	18940	4.9963	-	7470A	PPB	06 Nov 2018 11:56:56	U	SMPL
CCB05 - 1	CCB05	-29	-0.0431	-	7470A	PPB	06 Nov 2018 11:59:03	U	SMPL
J5771-02MS - 1	EO-01-110218-AMS	13646	3.5899	-	7470A	PPB	06 Nov 2018 12:01:11	U	SMPL
J5771-02MSD - 1	EO-01-110218-AMSD	14287	3.7602	-	7470A	PPB	06 Nov 2018 12:03:18	U	SMPL
J5771-04 - 1	EO-01-110218-B	-96	-0.0609	-	7470A	PPB	06 Nov 2018 12:05:26	U	SMPL
J5771-06 - 1	EO-01-110218-C	-45	-0.0473	-	7470A	PPB	06 Nov 2018 12:07:33	U	SMPL
J5778-05 - 1	OILY-GRAVEL	1	-0.0351	-	7470A	PPB	06 Nov 2018 12:09:41	U	SMPL
J5785-01 - 1	OIL-SP	-39	-0.0457	-	7470A	PPB	06 Nov 2018 12:11:48	U	SMPL
J5794-04 - 1	TP-12B-S	7	-0.0335	-	7470A	PPB	06 Nov 2018 12:13:57	U	SMPL
J5794-08 - 1	TP-11-S	13	-0.0319	-	7470A	PPB	06 Nov 2018 12:16:05	U	SMPL
J5794-12 - 1	TP-10B-S	-44	-0.0471	-	7470A	PPB	06 Nov 2018 12:18:14	U	SMPL
J5804-02 - 1	BS-DRUM-2	35	-0.0261	-	7470A	PPB	06 Nov 2018 12:20:21	U	SMPL
CCV06 - 1	CCV06	18684	4.9283	-	7470A	PPB	06 Nov 2018 12:22:29	U	SMPL
CCB06 - 1	CCB06	-5	-0.0367	-	7470A	PPB	06 Nov 2018 12:24:36	U	SMPL
PB114507BL - 1	PBW	-44	-0.0471	-	7470A	PPB	06 Nov 2018 12:26:43	U	SMPL
PB114507BS - 1	LCSW	13915	3.6613	-	7470A	PPB	06 Nov 2018 12:28:51	U	SMPL
J5778-07 - 1	OILY-WATER	428	0.0783	-	7470A	PPB	06 Nov 2018 12:30:58	U	SMPL
J5778-07DUP - 1	OILY-WATERDUP	503	0.0983	-	7470A	PPB	06 Nov 2018 12:33:06	U	SMPL
J5778-07MS - 1	OILY-WATERMS	14762	3.8863	-	7470A	PPB	06 Nov 2018 12:40:31	U	SMPL
J5778-07MSD - 1	OILY-WATERMSD	14888	3.9198	-	7470A	PPB	06 Nov 2018 12:42:38	U	SMPL
J5804-04 - 1	BS-DRUM-3	412	0.0741	-	7470A	PPB	06 Nov 2018 12:44:47	U	SMPL
PB114509BL - 1	PBW	75	-0.0154	-	7470A	PPB	06 Nov 2018 12:49:35	U	SMPL
PB114509BS - 1	LCSW	13843	3.6422	-	7470A	PPB	06 Nov 2018 12:54:28	U	SMPL
J5812-04 - 1	TP1-A	295	0.0430	-	7470A	PPB	06 Nov 2018 12:56:36	U	SMPL
CCV07 - 1	CCV07	18415	4.8568	-	7470A	PPB	06 Nov 2018 12:58:44	U	SMPL

LB99049 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Nov 2018 09:21:05

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB07 - 1	CCB07	-25	-0.0420	-7470A	PPB		06 Nov 2018 13:00:52	U	SMPL
J5812-04DUP - 1	TP1-ADUP	372	0.0635	-7470A	PPB		06 Nov 2018 13:05:42	U	SMPL
J5812-08 - 1	TP1-B	469	0.0892	-7470A	PPB		06 Nov 2018 13:12:05	U	SMPL
J5812-12 - 1	TP2-A	473	0.0903	-7470A	PPB		06 Nov 2018 13:14:14	U	SMPL
J5812-16 - 1	TP2-B	489	0.0945	-7470A	PPB		06 Nov 2018 13:16:21	U	SMPL
J5812-20 - 1	TP3-A	489	0.0945	-7470A	PPB		06 Nov 2018 13:18:30	U	SMPL
J5812-24 - 1	TP3-B	536	0.1070	-7470A	PPB		06 Nov 2018 13:20:40	U	SMPL
J5812-28 - 1	TP4-A	487	0.0940	-7470A	PPB		06 Nov 2018 13:22:49	U	SMPL
J5812-32 - 1	TP4-B	595	0.1227	-7470A	PPB		06 Nov 2018 13:24:58	U	SMPL
CCV08 - 1	CCV08	18441	4.8637	-7470A	PPB		06 Nov 2018 13:27:07	U	SMPL
CCB08 - 1	CCB08	-8	-0.0375	-7470A	PPB		06 Nov 2018 13:29:15	U	SMPL
J5815-02 - 1	HL-R37719-RT	492	0.0953	-7470A	PPB		06 Nov 2018 13:31:24	U	SMPL
J5815-04 - 1	HL-R47183-RT	578	0.1182	-7470A	PPB		06 Nov 2018 13:33:33	U	SMPL
J5815-06 - 1	HL-R25951-RT	522	0.1033	-7470A	PPB		06 Nov 2018 13:35:42	U	SMPL
J5816-04 - 1	TP-9-S	516	0.1017	-7470A	PPB		06 Nov 2018 13:37:50	U	SMPL
J5816-08 - 1	TP-4A-S	509	0.0999	-7470A	PPB		06 Nov 2018 13:39:58	U	SMPL
J5816-12 - 1	TP-4A-D	523	0.1036	-7470A	PPB		06 Nov 2018 13:42:06	U	SMPL
PB114533BL - 1	PBW	54	-0.0210	-7470A	PPB		06 Nov 2018 13:44:16	U	SMPL
PB114533BS - 1	LCSW	14540	3.8274	-7470A	PPB		06 Nov 2018 13:49:04	U	SMPL
J5804-03 - 1	BS-DRUM-3	-106	-0.0635	-7470A	PPB		06 Nov 2018 13:51:13	U	SMPL
J5804-03DUP - 1	BS-DRUM-3DUP	-76	-0.0556	-7470A	PPB		06 Nov 2018 13:53:21	U	SMPL
CCV09 - 1	CCV09	18892	4.9835	-7470A	PPB		06 Nov 2018 13:55:30	U	SMPL
CCB09 - 1	CCB09	-29	-0.0431	-7470A	PPB		06 Nov 2018 13:57:38	U	SMPL
J5804-03MS - 1	BS-DRUM-3MS	14702	3.8704	-7470A	PPB		06 Nov 2018 14:02:25	U	SMPL
J5804-03MSD - 1	BS-DRUM-3MSD	14837	3.9063	-7470A	PPB		06 Nov 2018 14:04:33	U	SMPL
PB114503TB - 1	PB114472TB	-63	-0.0521	-7470A	PPB		06 Nov 2018 14:06:41	U	SMPL
PB114506TB - 1	PB114443TB	40	-0.0247	-7470A	PPB		06 Nov 2018 14:08:49	U	SMPL
PB114507TB - 1	PB114452TB	30	-0.0274	-7470A	PPB		06 Nov 2018 14:10:57	U	SMPL
PB114509TB - 1	PB114484TB	184	0.0135	-7470A	PPB		06 Nov 2018 14:13:05	U	SMPL
J5812-04MS - 1	TP1-AMS	14377	3.7841	-7470A	PPB		06 Nov 2018 14:15:14	U	SMPL
J5812-04MSD - 1	TP1-AMSD	13705	3.6055	-7470A	PPB		06 Nov 2018 14:17:22	U	SMPL
CCV10 - 1	CCV10	18348	4.8390	-7470A	PPB		06 Nov 2018 14:19:31	U	SMPL
CCB10 - 1	CCB10	-67	-0.0532	-7470A	PPB		06 Nov 2018 14:21:39	U	SMPL
J5764-02LX5 - 1		14	-0.0316	-7470A	PPB		06 Nov 2018 14:23:46	U	SMPL
J5764-02A - 1		14480	3.8114	-7470A	PPB		06 Nov 2018 14:25:54	U	SMPL
J5771-02LX5 - 1		-9	-0.0378	-7470A	PPB		06 Nov 2018 14:28:03	U	SMPL
J5771-02A - 1		14242	3.7482	-7470A	PPB		06 Nov 2018 14:30:12	U	SMPL
J5778-07LX5 - 1		75	-0.0154	-7470A	PPB		06 Nov 2018 14:32:20	U	SMPL
J5778-07A - 1		15130	3.9841	-7470A	PPB		06 Nov 2018 14:34:28	U	SMPL
J5812-04LX5 - 1		26	-0.0285	-7470A	PPB		06 Nov 2018 14:36:35	U	SMPL
J5812-04A - 1		15540	4.0930	-7470A	PPB		06 Nov 2018 14:38:43	U	SMPL
J5804-03LX5 - 1		-40	-0.0460	-7470A	PPB		06 Nov 2018 14:40:51	U	SMPL
J5804-03A - 1		13885	3.6534	-7470A	PPB		06 Nov 2018 14:42:59	U	SMPL
CCV11 - 1	CCV11	18499	4.8791	-7470A	PPB		06 Nov 2018 14:45:09	U	SMPL
CCB11 - 1	CCB11	-38	-0.0455	-7470A	PPB		06 Nov 2018 14:47:17	U	SMPL