


245.1

LB 99117
INSTRUMENT ID: CV2

Linear

 μ Abs.:

36763

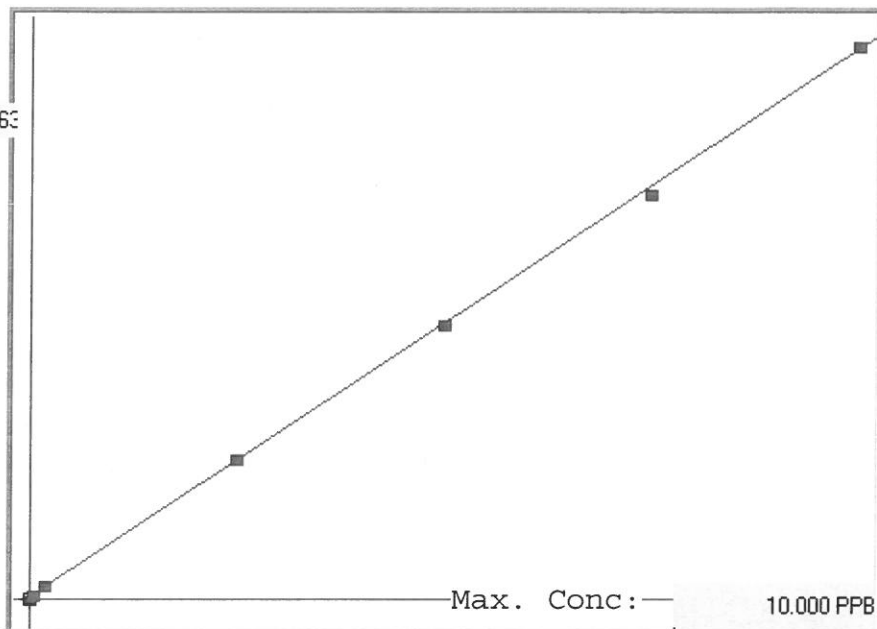

A= 0.0000e+000

B= 2.7480e-004

C= -2.7082e-002

Rho= 0.9998680

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.035	-0.035	-28	0.000	-28				
0.05	0.050	0.049	-0.001	278	0.0 %	278				
0.2	0.200	0.233	0.033	947	0.0 %	947				
2.5	2.500	2.544	0.044	9355	0.0 %	9355				
5.0	5.000	5.008	0.008	18322	0.0 %	18322				
7.5	7.500	7.375	-0.125	26938	0.0 %	26938				
10.0	10.000	10.075	0.075	36763	0.0 %	36763				

LB99117 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 09 Nov 2018 10:10:00

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-28	-	0.0000	245.1	PPB	09 Nov 2018 10:15:15	S	Std
0.05 - 1	50.05	278	-	0.0500	245.1	PPB	09 Nov 2018 10:25:17	S	Std
0.2 - 1	50.2	947	-	0.2000	245.1	PPB	09 Nov 2018 10:55:33	S	Std
2.5 - 1	52.5	9355	-	2.5000	245.1	PPB	09 Nov 2018 10:57:51	S	Std
5.0 - 1	55	18322	-	5.0000	245.1	PPB	09 Nov 2018 11:00:08	S	Std
7.5 - 1	57.5	26938	-	7.5000	245.1	PPB	09 Nov 2018 11:02:25	S	Std
10.0 - 1	510	36763	-	10.0000	245.1	PPB	09 Nov 2018 11:04:42	S	Std
ICV66 - 1	ICV66	14394	3.9284	-245.1		PPB	09 Nov 2018 11:10:04	U	SMPL
ICB66 - 1	ICB66	-50	-0.0408	-245.1		PPB	09 Nov 2018 11:14:55	U	SMPL
CCV40 - 1	CCV40	18523	5.0630	-245.1		PPB	09 Nov 2018 11:17:10	U	SMPL
CCB40 - 1	CCB40	-185	-0.0779	-245.1		PPB	09 Nov 2018 11:19:26	U	SMPL
CRA - 1	CRA	252	0.0422	-245.1		PPB	09 Nov 2018 11:21:43	U	SMPL
HighStd - 1	HighStd	35919	9.8434	-245.1		PPB	09 Nov 2018 11:23:58	U	SMPL
ChkStd - 1	ChkStd	26151	7.1592	-245.1		PPB	09 Nov 2018 11:26:14	U	SMPL
PB114648BL - 1	PBW	207	0.0298	-245.1		PPB	09 Nov 2018 11:31:14	U	SMPL
PB114648BS - 1	LCSW	12980	3.5398	-245.1		PPB	09 Nov 2018 11:33:30	U	SMPL
J5829-01 - 1	110518-SIDI-F-D-B	-194	-0.0804	-245.1		PPB	09 Nov 2018 11:35:47	U	SMPL
J5829-02 - 1	110518-SIDI-F-D-M	-136	-0.0645	-245.1		PPB	09 Nov 2018 11:38:04	U	SMPL
J5829-03 - 1	110518-SIDI-F-D-S	-136	-0.0645	-245.1		PPB	09 Nov 2018 11:40:22	U	SMPL
J5829-04 - 1	110518-SIDI-F-U-B	-127	-0.0620	-245.1		PPB	09 Nov 2018 11:42:40	U	SMPL
J5829-05 - 1	110518-SIDI-F-U-M	-138	-0.0650	-245.1		PPB	09 Nov 2018 11:44:56	U	SMPL
CCV41 - 1	CCV41	18478	5.0507	-245.1		PPB	09 Nov 2018 11:47:12	U	SMPL
CCB41 - 1	CCB41	-162	-0.0716	-245.1		PPB	09 Nov 2018 11:49:28	U	SMPL
J5829-06 - 1	110518-SIDI-F-U-S	-147	-0.0675	-245.1		PPB	09 Nov 2018 11:51:45	U	SMPL
J5829-07 - 1	110518-TIPC-E-D-M	-136	-0.0645	-245.1		PPB	09 Nov 2018 11:54:00	U	SMPL
J5829-08 - 1	110518-TIPC-E-U-M	-150	-0.0683	-245.1		PPB	09 Nov 2018 11:56:17	U	SMPL
J5829-09 - 1	110518-DBRI-E-D-B	-153	-0.0691	-245.1		PPB	09 Nov 2018 11:58:33	U	SMPL
J5829-10 - 1	110518-DBRI-E-D-M	-126	-0.0617	-245.1		PPB	09 Nov 2018 12:00:50	U	SMPL
J5829-11 - 1	110518-DBRI-E-D-S	-143	-0.0664	-245.1		PPB	09 Nov 2018 12:03:07	U	SMPL
J5829-12 - 1	110518-DBRI-E-U-B	-150	-0.0683	-245.1		PPB	09 Nov 2018 12:05:24	U	SMPL
J5829-13 - 1	110518-DBRI-E-U-M	-138	-0.0650	-245.1		PPB	09 Nov 2018 12:07:41	U	SMPL
J5829-14 - 1	110518-DBRI-E-U-S	-147	-0.0675	-245.1		PPB	09 Nov 2018 12:09:59	U	SMPL
J5829-14DUP - 1	110518-DBRI-E-U-SDUP	-123	-0.0609	-245.1		PPB	09 Nov 2018 12:12:15	U	SMPL
CCV42 - 1	CCV42	18834	5.1485	-245.1		PPB	09 Nov 2018 12:14:32	U	SMPL
CCB42 - 1	CCB42	-201	-0.0823	-245.1		PPB	09 Nov 2018 12:16:48	U	SMPL
J5829-14MS - 1	110518-DBRI-E-U-SMS	12497	3.4071	-245.1		PPB	09 Nov 2018 12:19:05	U	SMPL
J5829-14MSD - 1	110518-DBRI-E-U-SMSD	13323	3.6341	-245.1		PPB	09 Nov 2018 12:21:21	U	SMPL
PB114649BL - 1	PBW	-151	-0.0686	-245.1		PPB	09 Nov 2018 12:23:38	U	SMPL
J5851-01 - 1	110618-DBRI-F-D-B	-156	-0.0700	-245.1		PPB	09 Nov 2018 12:28:11	U	SMPL
J5851-02 - 1	110618-DBRI-F-D-M	-151	-0.0686	-245.1		PPB	09 Nov 2018 12:30:28	U	SMPL
J5851-03 - 1	110618-DBRI-F-D-S	-153	-0.0691	-245.1		PPB	09 Nov 2018 12:32:45	U	SMPL
J5851-04 - 1	110618-DBRI-F-U-B	-132	-0.0634	-245.1		PPB	09 Nov 2018 12:35:03	U	SMPL
J5851-05 - 1	110618-DBRI-F-U-M	-137	-0.0647	-245.1		PPB	09 Nov 2018 12:37:21	U	SMPL
J5851-06 - 1	110618-DBRI-F-U-S	-152	-0.0689	-245.1		PPB	09 Nov 2018 12:39:37	U	SMPL
CCV43 - 1	CCV43	18306	5.0034	-245.1		PPB	09 Nov 2018 12:41:54	U	SMPL
CCB43 - 1	CCB43	-175	-0.0752	-245.1		PPB	09 Nov 2018 12:44:10	U	SMPL
J5851-07 - 1	110618-JETT-F-D-B	-160	-0.0710	-245.1		PPB	09 Nov 2018 12:46:28	U	SMPL
J5851-08 - 1	110618-JETT-F-D-M	-137	-0.0647	-245.1		PPB	09 Nov 2018 12:48:44	U	SMPL
J5851-09 - 1	110618-JETT-F-D-S	-157	-0.0702	-245.1		PPB	09 Nov 2018 12:51:00	U	SMPL
J5851-10 - 1	110618-SIDI-F-D-B	-138	-0.0650	-245.1		PPB	09 Nov 2018 12:53:17	U	SMPL
J5851-11 - 1	110618-SIDI-F-D-M	-138	-0.0650	-245.1		PPB	09 Nov 2018 12:55:33	U	SMPL
J5851-12 - 1	110618-SIDI-F-D-S	-130	-0.0628	-245.1		PPB	09 Nov 2018 12:57:50	U	SMPL
J5851-13 - 1	110618-SIDI-F-U-B	-123	-0.0609	-245.1		PPB	09 Nov 2018 13:00:07	U	SMPL
J5851-14 - 1	110618-SIDI-F-U-M	-129	-0.0625	-245.1		PPB	09 Nov 2018 13:02:25	U	SMPL
J5851-15 - 1	110618-SIDI-F-U-S	-133	-0.0636	-245.1		PPB	09 Nov 2018 13:04:43	U	SMPL
J5851-16 - 1	110618-TIPC-E-D-M	-141	-0.0658	-245.1		PPB	09 Nov 2018 13:06:59	U	SMPL
CCV44 - 1	CCV44	18459	5.0454	-245.1		PPB	09 Nov 2018 13:09:15	U	SMPL
CCB44 - 1	CCB44	-176	-0.0754	-245.1		PPB	09 Nov 2018 13:11:32	U	SMPL
J5851-17 - 1	110618-TIPC-E-U-M	-146	-0.0672	-245.1		PPB	09 Nov 2018 13:13:49	U	SMPL
J5855-01 - 1	COMP	-99	-0.0543	-245.1		PPB	09 Nov 2018 13:16:05	U	SMPL
J5855-01DUP - 1	COMPDUP	-83	-0.0499	-245.1		PPB	09 Nov 2018 13:18:22	U	SMPL
J5855-01MS - 1	COMPMS	14972	4.0872	-245.1		PPB	09 Nov 2018 13:26:04	U	SMPL
J5855-01MSD - 1	COMPMSD	14726	4.0196	-245.1		PPB	09 Nov 2018 13:28:20	U	SMPL
PB114662BL - 1	PBW	-26	-0.0342	-245.1		PPB	09 Nov 2018 13:30:38	U	SMPL
PB114662BS - 1	LCSW	13885	3.7885	-245.1		PPB	09 Nov 2018 13:35:42	U	SMPL
J5881-01 - 1	110718-TIPC-F-D-B	-67	-0.0455	-245.1		PPB	09 Nov 2018 13:38:00	U	SMPL
J5881-02 - 1	110718-TIPC-F-D-S	33	-0.0180	-245.1		PPB	09 Nov 2018 13:40:17	U	SMPL
J5881-03 - 1	110718-TIPC-F-U-B	33	-0.0180	-245.1		PPB	09 Nov 2018 13:42:34	U	SMPL
CCV45 - 1	CCV45	18290	4.9990	-245.1		PPB	09 Nov 2018 13:44:50	U	SMPL
CCB45 - 1	CCB45	-178	-0.0760	-245.1		PPB	09 Nov 2018 13:47:07	U	SMPL
J5881-04 - 1	110718-TIPC-F-U-S	10	-0.0243	-245.1		PPB	09 Nov 2018 13:49:24	U	SMPL
J5881-05 - 1	110718-JETT-E-D-B	90	-0.0023	-245.1		PPB	09 Nov 2018 13:51:41	U	SMPL
J5881-06 - 1	110718-JETT-E-D-M	118	0.0053	-245.1		PPB	09 Nov 2018 13:53:57	U	SMPL
J5881-07 - 1	110718-JETT-E-D-S	209	0.0304	-245.1		PPB	09 Nov 2018 13:56:14	U	SMPL
J5881-10 - 1	110718-JETT-E-U-S	177	0.0216	-245.1		PPB	09 Nov 2018 14:03:04	U	SMPL
J5881-11 - 1	110718-DBRI-E-D-B	0	-0.0271	-245.1		PPB	09 Nov 2018 14:05:22	U	SMPL
J5881-12 - 1	110718-DBRI-E-D-M	32	-0.0183	-245.1		PPB	09 Nov 2018 14:07:39	U	SMPL
J5881-13 - 1	110718-DBRI-E-D-S	20	-0.0216	-245.1		PPB	09 Nov 2018 14:09:56	U	SMPL
CCV46 - 1	CCV46	18402	5.0298	-245.1		PPB	09 Nov 2018 14:12:13	U	SMPL
CCB46 - 1	CCB46	-55	-0.0422	-245.1		PPB	09 Nov 2018 14:14:30	U	SMPL
J5881-14 - 1	110718-DBRI-E-U-B	26	-0.0199	-245.1		PPB	09 Nov 2018 14:16:47	U	SMPL