


245.1

LB 99275
INSTRUMENT ID : CV1

Linear

 μ Abs.:

38437

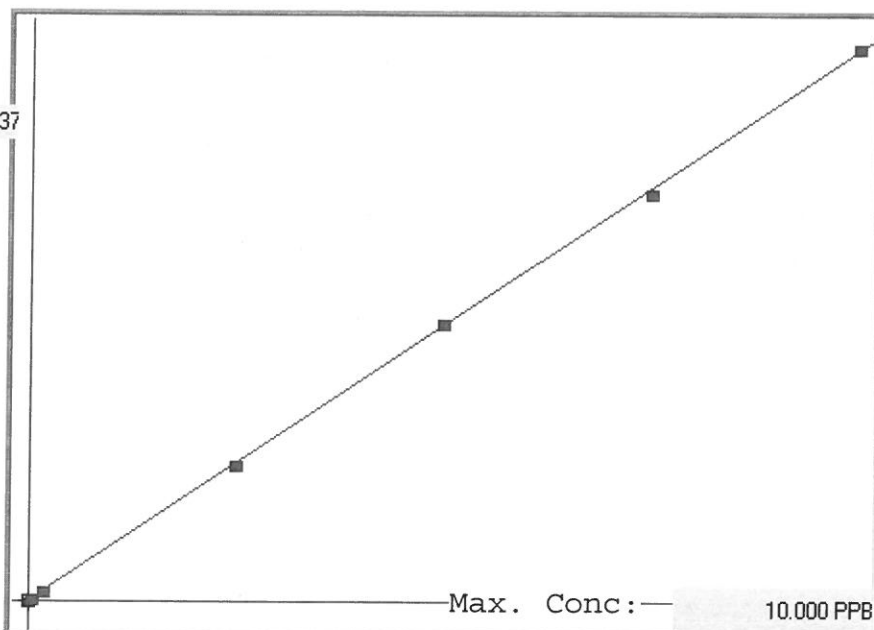

A= 0.0000e+000

B= 2.6128e-004

C= -4.9071e-003

Rho= 0.9999480

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.009	0.009	54	0.000	54				
0.05	0.050	0.062	0.012	256	0.0 %	256				
0.2	0.200	0.195	-0.005	767	0.0 %	767				
2.5	2.500	2.473	-0.027	9482	0.0 %	9482				
5.0	5.000	5.047	0.047	19334	0.0 %	19334				
7.5	7.500	7.426	-0.074	28442	0.0 %	28442				
10.0	10.000	10.038	0.038	38437	0.0 %	38437				

LB99275 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 16 Nov 2018 14:50:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	54	-	0.0000	245.1	PPB	16 Nov 2018 14:53:07	S	Std
0.05 - 1	50.05	256	-	0.0500	245.1	PPB	16 Nov 2018 14:55:26	S	Std
0.2 - 1	50.2	767	-	0.2000	245.1	PPB	16 Nov 2018 14:57:44	S	Std
2.5 - 1	52.5	9482	-	2.5000	245.1	PPB	16 Nov 2018 15:00:02	S	Std
5.0 - 1	55	19334	-	5.0000	245.1	PPB	16 Nov 2018 15:02:19	S	Std
7.5 - 1	57.5	28442	-	7.5000	245.1	PPB	16 Nov 2018 15:04:35	S	Std
10.0 - 1	510	38437	-	10.0000	245.1	PPB	16 Nov 2018 15:06:52	S	Std
ICV79 - 1	ICV79	14654	3.8239	-245.1		PPB	16 Nov 2018 15:09:53	U	SMPL
ICB79 - 1	ICB79	-41	-0.0156	-245.1		PPB	16 Nov 2018 15:12:08	U	SMPL
CCV32 - 1	CCV32	18985	4.9554	-245.1		PPB	16 Nov 2018 15:14:24	U	SMPL
CCB32 - 1	CCB32	-45	-0.0167	-245.1		PPB	16 Nov 2018 15:16:40	U	SMPL
CRA - 1	CRA	260	0.0630	-245.1		PPB	16 Nov 2018 15:18:56	U	SMPL
HighStd - 1	HighStd	37957	9.9124	-245.1		PPB	16 Nov 2018 15:21:13	U	SMPL
ChkStd - 1	ChkStd	26620	6.9503	-245.1		PPB	16 Nov 2018 15:23:29	U	SMPL
PB114872BL - 1	PBW	-107	-0.0329	-245.1		PPB	16 Nov 2018 15:25:47	U	SMPL
PB114872BS - 1	LCSW	13842	3.6117	-245.1		PPB	16 Nov 2018 15:28:05	U	SMPL
J5916-01 - 1	110918-SIDI-F-D-B	-148	-0.0436	-245.1		PPB	16 Nov 2018 15:30:22	U	SMPL
J5916-02 - 1	110918-SIDI-F-D-M	-71	-0.0235	-245.1		PPB	16 Nov 2018 15:32:39	U	SMPL
J5916-03 - 1	110918-SIDI-F-D-S	-65	-0.0219	-245.1		PPB	16 Nov 2018 15:34:56	U	SMPL
J5916-04 - 1	110918-SIDI-F-U-B	-50	-0.0180	-245.1		PPB	16 Nov 2018 15:37:15	U	SMPL
J5916-05 - 1	110918-SIDI-F-U-M	-71	-0.0235	-245.1		PPB	16 Nov 2018 15:39:30	U	SMPL
CCV33 - 1	CCV33	18743	4.8922	-245.1		PPB	16 Nov 2018 15:41:46	U	SMPL
CCB33 - 1	CCB33	-37	-0.0146	-245.1		PPB	16 Nov 2018 15:44:02	U	SMPL
J5916-06 - 1	110918-SIDI-F-U-S	-78	-0.0253	-245.1		PPB	16 Nov 2018 15:46:18	U	SMPL
J5916-07 - 1	110918-DBRI-F-D-B	-62	-0.0211	-245.1		PPB	16 Nov 2018 15:48:33	U	SMPL
J5916-08 - 1	110918-DBRI-F-D-M	-58	-0.0201	-245.1		PPB	16 Nov 2018 15:50:49	U	SMPL
J5916-09 - 1	110918-DBRI-F-D-S	-65	-0.0219	-245.1		PPB	16 Nov 2018 15:53:06	U	SMPL
J5916-10 - 1	110918-DBRI-F-U-B	-54	-0.0190	-245.1		PPB	16 Nov 2018 15:55:22	U	SMPL
J5916-11 - 1	110918-DBRI-F-U-M	-50	-0.0180	-245.1		PPB	16 Nov 2018 15:57:39	U	SMPL
J5916-12 - 1	110918-DBRI-F-U-S	-40	-0.0154	-245.1		PPB	16 Nov 2018 15:59:56	U	SMPL
J5916-13 - 1	110918-TIPC-F-D-B	-49	-0.0177	-245.1		PPB	16 Nov 2018 16:02:14	U	SMPL
J5916-14 - 1	110918-TIPC-F-D-S	-46	-0.0169	-245.1		PPB	16 Nov 2018 16:04:32	U	SMPL
J5916-15 - 1	110918-TIPC-F-U-B	-56	-0.0195	-245.1		PPB	16 Nov 2018 16:06:48	U	SMPL
CCV34 - 1	CCV34	19217	5.0161	-245.1		PPB	16 Nov 2018 16:09:05	U	SMPL
CCB34 - 1	CCB34	-26	-0.0117	-245.1		PPB	16 Nov 2018 16:11:22	U	SMPL
J5916-16 - 1	110918-TIPC-F-U-S	-82	-0.0263	-245.1		PPB	16 Nov 2018 16:13:38	U	SMPL
J5916-17 - 1	110918-JETT-F-D-B	-24	-0.0112	-245.1		PPB	16 Nov 2018 16:15:54	U	SMPL
J5916-18 - 1	110918-JETT-F-D-M	-55	-0.0193	-245.1		PPB	16 Nov 2018 16:18:11	U	SMPL
J5916-19 - 1	110918-JETT-F-D-S	-52	-0.0185	-245.1		PPB	16 Nov 2018 16:20:27	U	SMPL
J5916-20 - 1	110918-JETT-F-U-B	-36	-0.0143	-245.1		PPB	16 Nov 2018 16:22:44	U	SMPL
J5916-21 - 1	110918-JETT-F-U-M	-61	-0.0208	-245.1		PPB	16 Nov 2018 16:25:01	U	SMPL
J5916-22 - 1	110918-JETT-F-U-S	-53	-0.0188	-245.1		PPB	16 Nov 2018 16:27:18	U	SMPL
PB114873BL - 1	PBW	51	0.0084	-245.1		PPB	16 Nov 2018 16:29:36	U	SMPL
PB114873BS - 1	LCSW	13712	3.5777	-245.1		PPB	16 Nov 2018 16:31:54	U	SMPL
J5958-01 - 1	111318-SIDI-F-D-B	-121	-0.0365	-245.1		PPB	16 Nov 2018 16:34:10	U	SMPL
CCV35 - 1	CCV35	19060	4.9750	-245.1		PPB	16 Nov 2018 16:36:27	U	SMPL
CCB35 - 1	CCB35	-46	-0.0169	-245.1		PPB	16 Nov 2018 16:38:43	U	SMPL
J5958-02 - 1	111318-SIDI-F-D-S	-75	-0.0245	-245.1		PPB	16 Nov 2018 16:41:00	U	SMPL
J5958-03 - 1	111318-SIDI-F-U-B	-40	-0.0154	-245.1		PPB	16 Nov 2018 16:43:17	U	SMPL
J5958-04 - 1	111318-SIDI-F-U-S	-50	-0.0180	-245.1		PPB	16 Nov 2018 16:45:34	U	SMPL
J5959-01 - 1	111418-SIDI-E-D-B	-38	-0.0148	-245.1		PPB	16 Nov 2018 16:47:50	U	SMPL
J5959-02 - 1	111418-SIDI-E-D-S	-45	-0.0167	-245.1		PPB	16 Nov 2018 16:50:07	U	SMPL
J5959-03 - 1	111418-SIDI-E-U-B	-47	-0.0172	-245.1		PPB	16 Nov 2018 16:52:24	U	SMPL
J5959-04 - 1	111418-SIDI-E-U-S	-47	-0.0172	-245.1		PPB	16 Nov 2018 16:54:41	U	SMPL
J5959-05 - 1	111418-TIPC-E-D-M	-50	-0.0180	-245.1		PPB	16 Nov 2018 16:56:59	U	SMPL
J5959-06 - 1	111418-TIPC-E-U-M	-62	-0.0211	-245.1		PPB	16 Nov 2018 16:59:17	U	SMPL
J5959-06DUP - 1	111418-TIPC-E-U-MDUP	-50	-0.0180	-245.1		PPB	16 Nov 2018 17:01:33	U	SMPL
CCV36 - 1	CCV36	18991	4.9570	-245.1		PPB	16 Nov 2018 17:03:50	U	SMPL
CCB36 - 1	CCB36	-39	-0.0151	-245.1		PPB	16 Nov 2018 17:06:06	U	SMPL
J5959-06MS - 1	111418-TIPC-E-U-MMS	13416	3.5004	-245.1		PPB	16 Nov 2018 17:08:23	U	SMPL
J5959-06MSD - 1	111418-TIPC-E-U-MMSD	13457	3.5111	-245.1		PPB	16 Nov 2018 17:10:39	U	SMPL
J5959-06LX5 - 1		-25	-0.0114	-245.1		PPB	16 Nov 2018 17:12:55	U	SMPL
J5959-06A - 1		14564	3.8003	-245.1		PPB	16 Nov 2018 17:15:12	U	SMPL
CCV37 - 1	CCV37	19053	4.9732	-245.1		PPB	16 Nov 2018 17:17:29	U	SMPL
CCB37 - 1	CCB37	-38	-0.0148	-245.1		PPB	16 Nov 2018 17:19:46	U	SMPL