


7470A

LB99318
INSTRUMENT ID: CVZ

Linear

 μ Abs.:

34154

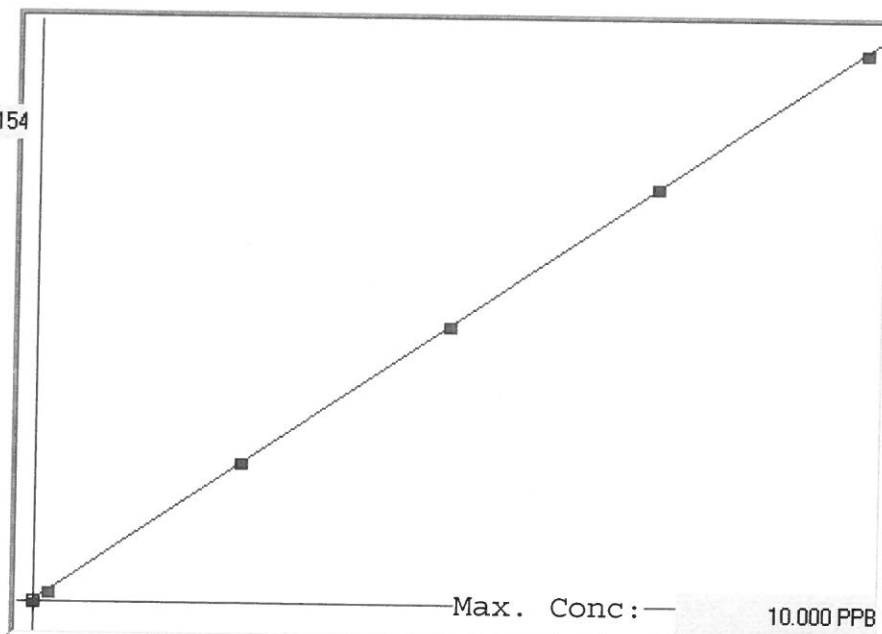

A= 0.0000e+000

B= 2.9246e-004

C= -1.9446e-002

Rho= 0.9999753

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.008	-0.008	40	0.000	40				
0.2	0.200	0.167	-0.033	637	0.0 %	637				
2.5	2.500	2.535	0.035	8736	0.0 %	8736				
5.0	5.000	5.020	0.020	17231	0.0 %	17231				
7.5	7.500	7.517	0.017	25768	0.0 %	25768				
10.0	10.000	9.969	-0.031	34154	0.0 %	34154				

LB99318 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 Nov 2018 11:04:38

Sample ID	Extended ID	µ Abs	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	40	-	0.00007470A	PPB	20 Nov 2018 11:09:01	S	Std
0.2 - 1	50.2	637	-	0.20007470A	PPB	20 Nov 2018 11:11:10	S	Std
2.5 - 1	52.1	8736	-	2.50007470A	PPB	20 Nov 2018 11:13:19	S	Std
5.0 - 1	55	17231	-	5.00007470A	PPB	20 Nov 2018 11:15:27	S	Std
7.5 - 1	57.5	25768	-	7.50007470A	PPB	20 Nov 2018 11:17:35	S	Std
10.0 - 1	510	34154	-	10.00007470A	PPB	20 Nov 2018 11:19:44	S	Std
ICV82 - 1	ICV82	14005	4.0764	-7470A	PPB	20 Nov 2018 11:22:33	U	SMPL
ICB82 - 1	ICB82	-51	-0.0344	-7470A	PPB	20 Nov 2018 11:24:39	U	SMPL
CCV52 - 1	CCV52	17412	5.0728	-7470A	PPB	20 Nov 2018 11:26:47	U	SMPL
CCB52 - 1	CCB52	-67	-0.0390	-7470A	PPB	20 Nov 2018 11:28:53	U	SMPL
CRA - 1	CRA	656	0.1724	-7470A	PPB	20 Nov 2018 11:31:01	U	SMPL
HighStd - 1	HighStd	34945	10.2004	-7470A	PPB	20 Nov 2018 11:33:07	U	SMPL
ChkStd - 1	ChkStd	24783	7.2285	-7470A	PPB	20 Nov 2018 11:35:14	U	SMPL
PB114935BL - 1	PBW	-144	-0.0616	-7470A	PPB	20 Nov 2018 11:37:24	U	SMPL
PB114935BS - 1	LCSW	13786	4.0123	-7470A	PPB	20 Nov 2018 11:39:32	U	SMPL
J5762-06 - 1	BU-03-111518	-57	-0.0361	-7470A	PPB	20 Nov 2018 11:41:40	U	SMPL
J5762-06DUP - 1	BU-03-111518DUP	16	-0.0148	-7470A	PPB	20 Nov 2018 11:43:48	U	SMPL
J5762-06MS - 1	BU-03-111518MS	13534	3.9386	-7470A	PPB	20 Nov 2018 11:45:56	U	SMPL
J5762-06MSD - 1	BU-03-111518MSD	13391	3.8968	-7470A	PPB	20 Nov 2018 11:48:05	U	SMPL
J5774-02 - 1	SU-04-111618	-55	-0.0355	-7470A	PPB	20 Nov 2018 11:50:13	U	SMPL
CCV53 - 1	CCV53	17969	5.2357	-7470A	PPB	20 Nov 2018 11:52:19	U	SMPL
CCB53 - 1	CCB53	-71	-0.0402	-7470A	PPB	20 Nov 2018 11:54:26	U	SMPL
J5954-01 - 1	OWS-1	45	-0.0063	-7470A	PPB	20 Nov 2018 11:56:33	U	SMPL
J5963-02 - 1	FS-OILY-STONE	37	-0.0086	-7470A	PPB	20 Nov 2018 11:58:40	U	SMPL
J5963-03 - 1	FS-OILY-PAD	119	0.0154	-7470A	PPB	20 Nov 2018 12:00:48	U	SMPL
J5963-04 - 1	FS-OIL	796	0.2133	-7470A	PPB	20 Nov 2018 12:02:55	U	SMPL
J5964-03 - 1	LR-RBR-200036	57	-0.0028	-7470A	PPB	20 Nov 2018 12:05:03	U	SMPL
J5964-06 - 1	LR-RBR-200029	61	-0.0016	-7470A	PPB	20 Nov 2018 12:07:10	U	SMPL
J5975-02 - 1	VB44949	78	0.0034	-7470A	PPB	20 Nov 2018 12:09:19	U	SMPL
J5983-01 - 1	OILY-DEBRIS-A	54	-0.0037	-7470A	PPB	20 Nov 2018 12:11:27	U	SMPL
J5983-03 - 1	OILY-DEBRIS-B	70	0.0010	-7470A	PPB	20 Nov 2018 12:13:36	U	SMPL
J5989-02 - 1	ES-RO-343	49	-0.0051	-7470A	PPB	20 Nov 2018 12:15:43	U	SMPL
CCV54 - 1	CCV54	17480	5.0927	-7470A	PPB	20 Nov 2018 12:17:49	U	SMPL
CCB54 - 1	CCB54	-67	-0.0390	-7470A	PPB	20 Nov 2018 12:19:56	U	SMPL
J5991-02 - 1	WS-RO-358	32	-0.0101	-7470A	PPB	20 Nov 2018 12:22:04	U	SMPL
PB114936BL - 1	PBW	61	-0.0016	-7470A	PPB	20 Nov 2018 12:24:11	U	SMPL
PB114936BS - 1	LCSW	14259	4.1507	-7470A	PPB	20 Nov 2018 12:26:19	U	SMPL
J5975-04 - 1	VB44949	3	-0.0186	-7470A	PPB	20 Nov 2018 12:28:26	U	SMPL
J5976-02 - 1	OILY-WATER	52	-0.0042	-7470A	PPB	20 Nov 2018 12:30:34	U	SMPL
J5976-02DUP - 1	OILY-WATERDUP	74	0.0022	-7470A	PPB	20 Nov 2018 12:32:41	U	SMPL
J5976-02MS - 1	OILY-WATERMS	13407	3.9015	-7470A	PPB	20 Nov 2018 12:34:49	U	SMPL
J5976-02MSD - 1	OILY-WATERMSD	13288	3.8667	-7470A	PPB	20 Nov 2018 12:36:58	U	SMPL
J5980-02 - 1	TS	9	-0.0221	-7470A	PPB	20 Nov 2018 12:39:07	U	SMPL
PB114937BL - 1	PBW	48	-0.0054	-7470A	PPB	20 Nov 2018 12:41:14	U	SMPL
CCV55 - 1	CCV55	17507	5.1006	-7470A	PPB	20 Nov 2018 12:43:22	U	SMPL
CCB55 - 1	CCB55	-34	-0.0294	-7470A	PPB	20 Nov 2018 12:45:29	U	SMPL
PB114937BS - 1	LCSW	12593	3.6634	-7470A	PPB	20 Nov 2018 12:47:37	U	SMPL
J5993-10 - 1	SPLP-LEACHATE-AMENDED-WCC-1-COMPOSITE	244	0.0519	-7470A	PPB	20 Nov 2018 12:49:44	U	SMPL
J5993-10DUP - 1	SPLP-LEACHATE-AMENDED-WCC-1-COMPOSITEDUP	23	-0.0127	-7470A	PPB	20 Nov 2018 12:51:52	U	SMPL
J5993-10MS - 1	SPLP-LEACHATE-AMENDED-WCC-1-COMPOSITEMS	13902	4.0463	-7470A	PPB	20 Nov 2018 12:54:00	U	SMPL
J5993-10MSD - 1	SPLP-LEACHATE-AMENDED-WCC-1-COMPOSITMSD	14444	4.2048	-7470A	PPB	20 Nov 2018 12:56:08	U	SMPL
J5993-11 - 1	SPLP-LEACHATE-AMENDED-WCC-2-COMPOSITE	-21	-0.0256	-7470A	PPB	20 Nov 2018 12:58:16	U	SMPL
J5993-12 - 1	SPLP-LEACHATE-AMENDED-WCC-3-COMPOSITE	32	-0.0101	-7470A	PPB	20 Nov 2018 13:00:24	U	SMPL
PB114947BL - 1	PBW	53	-0.0039	-7470A	PPB	20 Nov 2018 13:02:32	U	SMPL
PB114947BS - 1	LCSW	13868	4.0363	-7470A	PPB	20 Nov 2018 13:04:40	U	SMPL
J5975-03 - 1	VB44949	5089	1.4689	-7470A	PPB	20 Nov 2018 13:06:48	U	SMPL
CCV56 - 1	CCV56	16927	4.9309	-7470A	PPB	20 Nov 2018 13:08:56	U	SMPL
CCB56 - 1	CCB56	8	-0.0171	-7470A	PPB	20 Nov 2018 13:11:04	U	SMPL
J5975-03DUP - 1	VB44949DUP	5117	1.4770	-7470A	PPB	20 Nov 2018 13:13:12	U	SMPL
J5975-03MS - 1	VB44949MS	16263	4.7368	-7470A	PPB	20 Nov 2018 13:15:20	U	SMPL
J5975-03MSD - 1	VB44949MSD	16327	4.7556	-7470A	PPB	20 Nov 2018 13:17:28	U	SMPL
J5976-01 - 1	OILY-WATER	1023	0.2797	-7470A	PPB	20 Nov 2018 13:19:36	U	SMPL
J5980-01 - 1	TS	1	-0.0192	-7470A	PPB	20 Nov 2018 13:21:44	U	SMPL
J5993-07 - 1	20180899-FIELD-BLANK	39	-0.0080	-7470A	PPB	20 Nov 2018 13:23:52	U	SMPL
J5994-01 - 1	20180923-SITE-WATER	-12	-0.0230	-7470A	PPB	20 Nov 2018 13:26:00	U	SMPL
J5994-02 - 1	20180924-FIELD-BLANK	-27	-0.0273	-7470A	PPB	20 Nov 2018 13:28:08	U	SMPL
PB114935TB - 1	PB114845TB	82	0.0045	-7470A	PPB	20 Nov 2018 13:30:16	U	SMPL
PB114936TB - 1	PB114896TB	74	0.0022	-7470A	PPB	20 Nov 2018 13:32:24	U	SMPL
CCV57 - 1	CCV57	17318	5.0453	-7470A	PPB	20 Nov 2018 13:34:32	U	SMPL
CCB57 - 1	CCB57	1	-0.0192	-7470A	PPB	20 Nov 2018 13:36:40	U	SMPL
PB114937TB - 1	PB114900TB	124	0.0168	-7470A	PPB	20 Nov 2018 13:38:48	U	SMPL
J5762-06LX5 - 1		39	-0.0080	-7470A	PPB	20 Nov 2018 13:40:56	U	SMPL
J5762-06A - 1		14071	4.0957	-7470A	PPB	20 Nov 2018 13:43:04	U	SMPL
J5976-02LX5 - 1		-13	-0.0232	-7470A	PPB	20 Nov 2018 13:45:12	U	SMPL
J5976-02A - 1		14273	4.1548	-7470A	PPB	20 Nov 2018 13:47:20	U	SMPL
J5993-10LX5 - 1		-33	-0.0291	-7470A	PPB	20 Nov 2018 13:49:28	U	SMPL
J5993-10A - 1		14480	4.2153	-7470A	PPB	20 Nov 2018 13:51:36	U	SMPL
J5975-03LX5 - 1		949	0.2581	-7470A	PPB	20 Nov 2018 13:53:44	U	SMPL
J5975-03A - 1		18180	5.2974	-7470A	PPB	20 Nov 2018 13:55:52	U	SMPL
CCV58 - 1	CCV58	17223	5.0175	-7470A	PPB	20 Nov 2018 13:58:00	U	SMPL
CCB58 - 1	CCB58	-27	-0.0273	-7470A	PPB	20 Nov 2018 14:00:08	U	SMPL