


7470A

L399339

INSTRUMENT ID: CXL

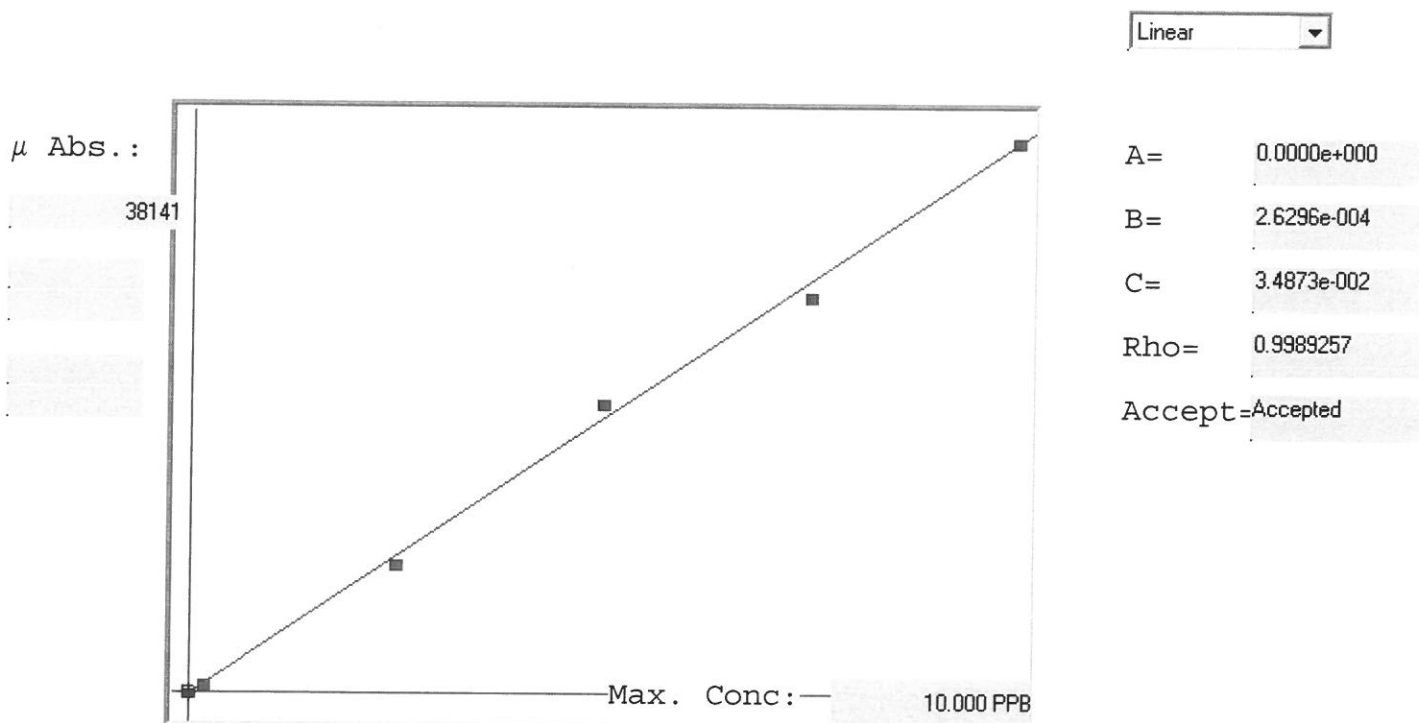

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.032	0.032	-10	0.000	-10				
0.2	0.200	0.198	-0.002	620	0.0 %	620				
2.5	2.500	2.376	-0.124	8902	0.0 %	8902				
5.0	5.000	5.293	0.293	19994	0.0 %	19994				
7.5	7.500	7.237	-0.263	27388	0.0 %	27388				
10.0	10.000	10.065	0.065	38141	0.0 %	38141				

LB99339 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Nov 2018 09:46:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-10	-	0.0000	7470A	PPB	21 Nov 2018 10:16:19	S	Std
0.2 - 1	50.2	620	-	0.2000	7470A	PPB	21 Nov 2018 10:18:28	S	Std
2.5 - 1	52.5	8902	-	2.5000	7470A	PPB	21 Nov 2018 10:20:37	S	Std
5.0 - 1	55	19994	-	5.0000	7470A	PPB	21 Nov 2018 10:22:46	S	Std
7.5 - 1	57.5	27388	-	7.5000	7470A	PPB	21 Nov 2018 10:24:54	S	Std
10.0 - 1	57.5	38141	-	10.0000	7470A	PPB	21 Nov 2018 10:31:53	S	Std
ICV84 - 1	ICV84	14184	3.7648	-7470A	PPB	21 Nov 2018 10:34:28	U	SMPL	
ICB84 - 1	ICB84	-111	0.0057	-7470A	PPB	21 Nov 2018 10:36:34	U	SMPL	
CCV65 - 1	CCV65	19487	5.1592	-7470A	PPB	21 Nov 2018 10:38:41	U	SMPL	
CCB65 - 1	CCB65	-112	0.0054	-7470A	PPB	21 Nov 2018 10:40:48	U	SMPL	
CRA - 1	CRA	601	0.1929	-7470A	PPB	21 Nov 2018 10:42:55	U	SMPL	
HighStd - 1	HighStd	37794	9.9733	-7470A	PPB	21 Nov 2018 10:45:01	U	SMPL	
ChkStd - 1	ChkStd	25374	6.7073	-7470A	PPB	21 Nov 2018 10:47:08	U	SMPL	
PB114995BL - 1	PBW	-158	-0.0067	-7470A	PPB	21 Nov 2018 10:49:17	U	SMPL	
PB114995BS - 1	LCSW	14117	3.7471	-7470A	PPB	21 Nov 2018 10:51:25	U	SMPL	
J5763-02 - 1	HR-06-111918-A	-97	0.0094	-7470A	PPB	21 Nov 2018 10:53:33	U	SMPL	
J5763-02DUP - 1	HR-06-111918-ADUP	-38	0.0249	-7470A	PPB	21 Nov 2018 10:55:41	U	SMPL	
J5763-02MS - 1	HR-06-111918-AMS	13336	3.5418	-7470A	PPB	21 Nov 2018 10:57:50	U	SMPL	
J5763-02MSD - 1	HR-06-111918-AMSD	13473	3.5778	-7470A	PPB	21 Nov 2018 10:59:58	U	SMPL	
J5763-04 - 1	HR-06-111918-B	-92	0.0107	-7470A	PPB	21 Nov 2018 11:02:05	U	SMPL	
CCV66 - 1	CCV66	19477	5.1566	-7470A	PPB	21 Nov 2018 11:04:12	U	SMPL	
CCB66 - 1	CCB66	-85	0.0125	-7470A	PPB	21 Nov 2018 11:06:19	U	SMPL	
J5775-02 - 1	TR-05-111918	-51	0.0215	-7470A	PPB	21 Nov 2018 11:08:26	U	SMPL	
J5999-01 - 1	SSSI-1114-S-TCLP-2	-26	0.0280	-7470A	PPB	21 Nov 2018 11:10:33	U	SMPL	
J5999-02 - 1	SSSI-1114-S-TCLP-3	-28	0.0275	-7470A	PPB	21 Nov 2018 11:12:40	U	SMPL	
J5999-03 - 1	SSSI-1114-S-TCLP-4	-35	0.0257	-7470A	PPB	21 Nov 2018 11:14:47	U	SMPL	
J6000-02 - 1	FS-12072-11929	-34	0.0259	-7470A	PPB	21 Nov 2018 11:16:54	U	SMPL	
J6006-02 - 1	RS-CON-WALL-1	-37	0.0251	-7470A	PPB	21 Nov 2018 11:19:02	U	SMPL	
J6006-04 - 1	RS-CON-WALL-2	-36	0.0254	-7470A	PPB	21 Nov 2018 11:21:10	U	SMPL	
J6006-06 - 1	RS-CON-FLOOR	-47	0.0225	-7470A	PPB	21 Nov 2018 11:23:18	U	SMPL	
J6010-03 - 1	FS-RT3786	-27	0.0278	-7470A	PPB	21 Nov 2018 11:25:27	U	SMPL	
CCV67 - 1	CCV67	19625	5.1955	-7470A	PPB	21 Nov 2018 11:27:34	U	SMPL	
CCB67 - 1	CCB67	-93	0.0104	-7470A	PPB	21 Nov 2018 11:29:41	U	SMPL	
PB114995TB - 1	PB114951TB	10	0.0375	-7470A	PPB	21 Nov 2018 11:31:48	U	SMPL	
J5763-02LX5 - 1		-37	0.0251	-7470A	PPB	21 Nov 2018 11:33:55	U	SMPL	
J5763-02A - 1		15396	4.0835	-7470A	PPB	21 Nov 2018 11:36:03	U	SMPL	
CCV68 - 1	CCV68	19326	5.1169	-7470A	PPB	21 Nov 2018 11:38:10	U	SMPL	
CCB68 - 1	CCB68	-97	0.0094	-7470A	PPB	21 Nov 2018 11:40:17	U	SMPL	