

L399358


245.1

INSTRUMENT ID: CV1

Linear

μ Abs.:

36853

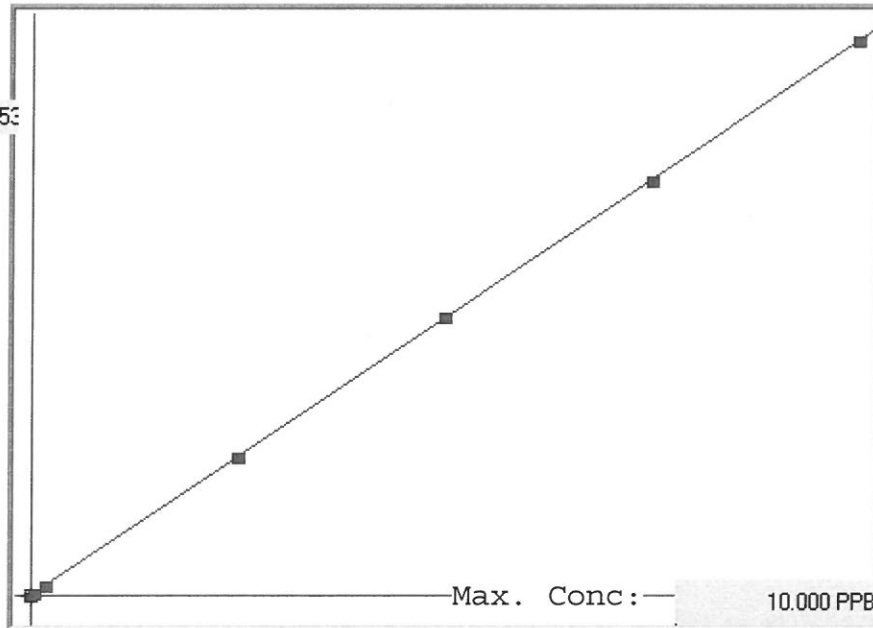

A= 0.0000e+000

B= 2.7124e-004

C= -2.0741e-003

Rho= 0.9999907

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.007	0.007	34	0.000	34				
0.05	0.050	0.049	-0.001	187	0.0 %	187				
0.2	0.200	0.184	-0.016	686	0.0 %	686				
2.5	2.500	2.494	-0.006	9204	0.0 %	9204				
5.0	5.000	5.035	0.035	18571	0.0 %	18571				
7.5	7.500	7.487	-0.013	27609	0.0 %	27609				
10.0	10.000	9.994	-0.006	36853	0.0 %	36853				

LB99358 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 21 Nov 2018 14:30:14

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	34	-	0.0000	245.1	PPB	21 Nov 2018 14:37:58	S	Std
0.05 - 1	50.05	187	-	0.0500	245.1	PPB	21 Nov 2018 14:40:15	S	Std
0.2 - 1	50.2	686	-	0.2000	245.1	PPB	21 Nov 2018 14:42:33	S	Std
2.5 - 1	52.5	9204	-	2.5000	245.1	PPB	21 Nov 2018 14:44:51	S	Std
5.0 - 1	55	18571	-	5.0000	245.1	PPB	21 Nov 2018 14:47:08	S	Std
7.5 - 1	57.5	27609	-	7.5000	245.1	PPB	21 Nov 2018 14:49:25	S	Std
10.0 - 1	510	36853	-	10.0000	245.1	PPB	21 Nov 2018 15:02:06	S	Std
ICV86 - 1	ICV86	14622	3.9640	-245.1	PPB	21 Nov 2018 15:04:54	U	SMPL	
ICB86 - 1	ICB86	-129	-0.0371	-245.1	PPB	21 Nov 2018 15:07:10	U	SMPL	
CCV74 - 1	CCV74	18403	4.9896	-245.1	PPB	21 Nov 2018 15:09:26	U	SMPL	
CCB74 - 1	CCB74	-128	-0.0368	-245.1	PPB	21 Nov 2018 15:11:42	U	SMPL	
CRA - 1	CRA	161	0.0416	-245.1	PPB	21 Nov 2018 15:13:58	U	SMPL	
HighStd - 1	HighStd	36690	9.9498	-245.1	PPB	21 Nov 2018 15:16:14	U	SMPL	
ChkStd - 1	ChkStd	25500	6.9146	-245.1	PPB	21 Nov 2018 15:18:30	U	SMPL	
PB115011BL - 1	PBW	-163	-0.0463	-245.1	PPB	21 Nov 2018 15:20:49	U	SMPL	
PB115011BS - 1	LCSW	15176	4.1143	-245.1	PPB	21 Nov 2018 15:25:40	U	SMPL	
J5985-01 - 1	111518-DBRI-E-D-B	-183	-0.0517	-245.1	PPB	21 Nov 2018 15:27:57	U	SMPL	
J5985-02 - 1	111518-DBRI-E-D-S	-115	-0.0333	-245.1	PPB	21 Nov 2018 15:30:14	U	SMPL	
J5985-03 - 1	111518-DBRI-E-U-B	-101	-0.0295	-245.1	PPB	21 Nov 2018 15:32:32	U	SMPL	
J5985-04 - 1	111518-DBRI-E-U-S	-97	-0.0284	-245.1	PPB	21 Nov 2018 15:34:49	U	SMPL	
J5985-05 - 1	111518-TIPC-E-D-M	-102	-0.0297	-245.1	PPB	21 Nov 2018 15:37:05	U	SMPL	
CCV75 - 1	CCV75	18401	4.9890	-245.1	PPB	21 Nov 2018 15:39:21	U	SMPL	
CCB75 - 1	CCB75	-118	-0.0341	-245.1	PPB	21 Nov 2018 15:41:37	U	SMPL	
J5985-06 - 1	111518-TIPC-E-U-M	-116	-0.0335	-245.1	PPB	21 Nov 2018 15:43:54	U	SMPL	
J5985-07 - 1	111518-JETT-E-D-B	-90	-0.0265	-245.1	PPB	21 Nov 2018 15:46:10	U	SMPL	
J5985-08 - 1	111518-JETT-E-D-M	-97	-0.0284	-245.1	PPB	21 Nov 2018 15:48:26	U	SMPL	
J5985-09 - 1	111518-JETT-E-D-S	-97	-0.0284	-245.1	PPB	21 Nov 2018 15:50:43	U	SMPL	
J5985-10 - 1	111518-JETT-E-U-B	-87	-0.0257	-245.1	PPB	21 Nov 2018 15:52:59	U	SMPL	
J5985-11 - 1	111518-JETT-E-U-M	-102	-0.0297	-245.1	PPB	21 Nov 2018 15:55:16	U	SMPL	
J5985-12 - 1	111518-JETT-E-U-S	-107	-0.0311	-245.1	PPB	21 Nov 2018 15:57:33	U	SMPL	
J5985-12DUP - 1	111518-JETT-E-U-SDUP	-94	-0.0276	-245.1	PPB	21 Nov 2018 15:59:51	U	SMPL	
J5985-12MS - 1	111518-JETT-E-U-SMS	15280	4.1425	-245.1	PPB	21 Nov 2018 16:02:09	U	SMPL	
J5985-12MSD - 1	111518-JETT-E-U-SMSD	15261	4.1373	-245.1	PPB	21 Nov 2018 16:04:25	U	SMPL	
CCV76 - 1	CCV76	17894	4.8515	-245.1	PPB	21 Nov 2018 16:06:42	U	SMPL	
CCB76 - 1	CCB76	-119	-0.0344	-245.1	PPB	21 Nov 2018 16:08:59	U	SMPL	
PB115012BL - 1	PBW	-28	-0.0097	-245.1	PPB	21 Nov 2018 16:11:15	U	SMPL	
PB115012BS - 1	LCSW	14841	4.0234	-245.1	PPB	21 Nov 2018 16:13:31	U	SMPL	
J6023-01 - 1	111918-JETT-E-D-B	-116	-0.0335	-245.1	PPB	21 Nov 2018 16:15:48	U	SMPL	
J6023-02 - 1	111918-JETT-E-D-M	-76	-0.0227	-245.1	PPB	21 Nov 2018 16:18:05	U	SMPL	
J6023-03 - 1	111918-JETT-E-D-S	-66	-0.0200	-245.1	PPB	21 Nov 2018 16:20:22	U	SMPL	
J6023-04 - 1	111918-JETT-E-U-B	-52	-0.0162	-245.1	PPB	21 Nov 2018 16:22:39	U	SMPL	
J6023-05 - 1	111918-JETT-E-U-M	-55	-0.0170	-245.1	PPB	21 Nov 2018 16:24:56	U	SMPL	
J6023-06 - 1	111918-JETT-E-U-S	-86	-0.0254	-245.1	PPB	21 Nov 2018 16:27:13	U	SMPL	
J6023-07 - 1	111918-DBRI-E-D-M	-74	-0.0221	-245.1	PPB	21 Nov 2018 16:29:31	U	SMPL	
J6023-08 - 1	111918-DBRI-E-U-M	-87	-0.0257	-245.1	PPB	21 Nov 2018 16:31:48	U	SMPL	
CCV77 - 1	CCV77	18125	4.9142	-245.1	PPB	21 Nov 2018 16:34:04	U	SMPL	
CCB77 - 1	CCB77	-100	-0.0292	-245.1	PPB	21 Nov 2018 16:36:21	U	SMPL	
J6023-09 - 1	111918-TIPC-E-D-B	-94	-0.0276	-245.1	PPB	21 Nov 2018 16:38:37	U	SMPL	
J6023-10 - 1	111918-TIPC-E-D-S	-76	-0.0227	-245.1	PPB	21 Nov 2018 16:40:54	U	SMPL	
J6023-11 - 1	111918-TIPC-E-U-B	-66	-0.0200	-245.1	PPB	21 Nov 2018 16:43:11	U	SMPL	
J6023-12 - 1	111918-TIPC-E-U-S	-78	-0.0232	-245.1	PPB	21 Nov 2018 16:45:27	U	SMPL	
J6023-13 - 1	111918-CHDE-E-D-B	-79	-0.0235	-245.1	PPB	21 Nov 2018 16:47:44	U	SMPL	
J6023-14 - 1	111918-CHDE-E-D-S	-77	-0.0230	-245.1	PPB	21 Nov 2018 16:50:02	U	SMPL	
J6023-15 - 1	111918-CHDE-E-U-B	-78	-0.0232	-245.1	PPB	21 Nov 2018 16:52:19	U	SMPL	
J6023-16 - 1	111918-CHDE-E-U-S	-79	-0.0235	-245.1	PPB	21 Nov 2018 16:54:37	U	SMPL	
J6023-16DUP - 1	111918-CHDE-E-U-SDUP	-80	-0.0238	-245.1	PPB	21 Nov 2018 16:56:55	U	SMPL	
J6023-16MS - 1	111918-CHDE-E-U-SMS	13406	3.6342	-245.1	PPB	21 Nov 2018 16:59:11	U	SMPL	
CCV78 - 1	CCV78	18265	4.9522	-245.1	PPB	21 Nov 2018 17:01:28	U	SMPL	
CCB78 - 1	CCB78	-116	-0.0335	-245.1	PPB	21 Nov 2018 17:03:44	U	SMPL	
J6023-16MSD - 1	111918-CHDE-E-U-SMSD	13702	3.7145	-245.1	PPB	21 Nov 2018 17:06:01	U	SMPL	
J5985-12LX5 - 1		-102	-0.0297	-245.1	PPB	21 Nov 2018 17:08:17	U	SMPL	
J5985-12A - 1		14356	3.8919	-245.1	PPB	21 Nov 2018 17:10:33	U	SMPL	
J6023-16LX5 - 1		-101	-0.0295	-245.1	PPB	21 Nov 2018 17:12:50	U	SMPL	
J6023-16A - 1		13872	3.7606	-245.1	PPB	21 Nov 2018 17:15:06	U	SMPL	
CCV79 - 1	CCV79	17685	4.7948	-245.1	PPB	21 Nov 2018 17:17:23	U	SMPL	
CCB79 - 1	CCB79	-141	-0.0403	-245.1	PPB	21 Nov 2018 17:19:40	U	SMPL	