

LB 99523


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

37581

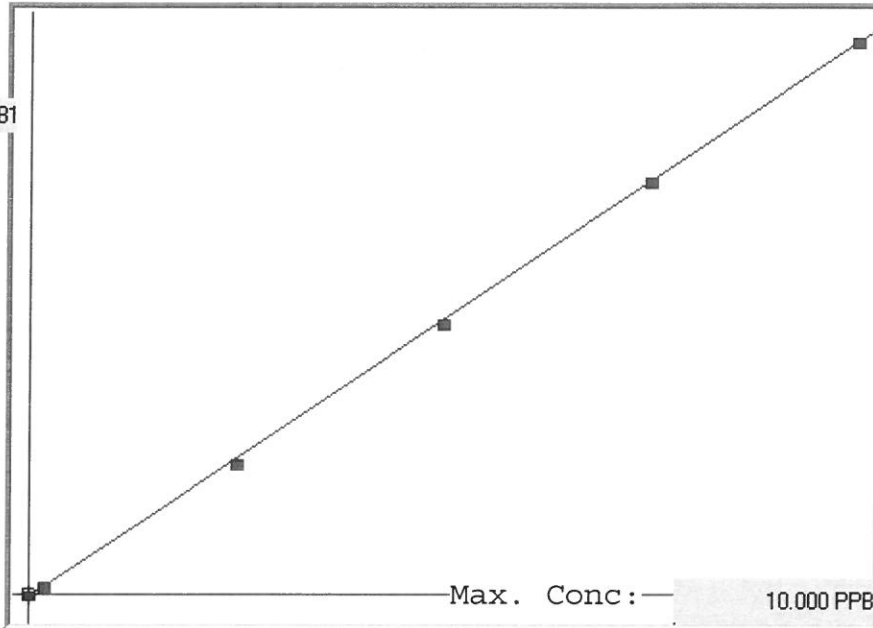

A= 0.0000e+000

B= 2.6533e-004

C= 5.5765e-002

Rho= 0.9999403

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.041	0.041	-54	0.000	-54				
0.2	0.200	0.228	0.028	648	0.0 %	648				
2.5	2.500	2.437	-0.063	8976	0.0 %	8976				
5.0	5.000	4.951	-0.049	18450	0.0 %	18450				
7.5	7.500	7.515	0.015	28113	0.0 %	28113				
10.0	10.000	10.027	0.027	37581	0.0 %	37581				

LB99523 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Dec 2018 10:35:35

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-54	-	0.0000	7470A	PPB	03 Dec 2018 10:40:09	S	Std
0.2 - 1	50.2	648	-	0.2000	7470A	PPB	03 Dec 2018 10:42:18	S	Std
2.5 - 1	52.5	8976	-	2.5000	7470A	PPB	03 Dec 2018 10:44:26	S	Std
5.0 - 1	55	18450	-	5.0000	7470A	PPB	03 Dec 2018 10:46:34	S	Std
7.5 - 1	57.5	28113	-	7.5000	7470A	PPB	03 Dec 2018 10:48:42	S	Std
10.0 - 1	57.1	37581	-	10.0000	7470A	PPB	03 Dec 2018 10:53:13	S	Std
ICV01 - 1	ICV01	14926	4.0161	-	7470A	PPB	03 Dec 2018 10:55:50	U	SMPL
ICB01 - 1	ICB01	-162	0.0128	-	7470A	PPB	03 Dec 2018 10:57:57	U	SMPL
CCV47 - 1	CCV47	19832	5.3178	-	7470A	PPB	03 Dec 2018 11:00:04	U	SMPL
CCB47 - 1	CCB47	-148	0.0165	-	7470A	PPB	03 Dec 2018 11:02:10	U	SMPL
CRA - 1	CRA	655	0.2296	-	7470A	PPB	03 Dec 2018 11:04:17	U	SMPL
HighStd - 1	HighStd	37569	10.0241	-	7470A	PPB	03 Dec 2018 11:06:23	U	SMPL
ChkStd - 1	ChkStd	26367	7.0518	-	7470A	PPB	03 Dec 2018 11:08:30	U	SMPL
PB115228BL - 1	PBW	-161	0.0130	-	7470A	PPB	03 Dec 2018 11:10:38	U	SMPL
PB115228BS - 1	LCSW	14568	3.9211	-	7470A	PPB	03 Dec 2018 11:12:45	U	SMPL
J5761-02 - 1	AU-06-112918	-144	0.0176	-	7470A	PPB	03 Dec 2018 11:14:53	U	SMPL
J5761-02DUP - 1	AU-06-112918DUP	-44	0.0441	-	7470A	PPB	03 Dec 2018 11:17:01	U	SMPL
J5761-02MS - 1	AU-06-112918MS	13924	3.7503	-	7470A	PPB	03 Dec 2018 11:19:09	U	SMPL
J5761-02MSD - 1	AU-06-112918MSD	13715	3.6948	-	7470A	PPB	03 Dec 2018 11:21:18	U	SMPL
J5761-04 - 1	AU-05-112918	-67	0.0380	-	7470A	PPB	03 Dec 2018 11:23:25	U	SMPL
CCV48 - 1	CCV48	18864	5.0610	-	7470A	PPB	03 Dec 2018 11:25:31	U	SMPL
CCB48 - 1	CCB48	-130	0.0213	-	7470A	PPB	03 Dec 2018 11:27:38	U	SMPL
J5762-08 - 1	BU-02-112918	-45	0.0438	-	7470A	PPB	03 Dec 2018 11:29:45	U	SMPL
J5765-06 - 1	NB-07-112918	-51	0.0422	-	7470A	PPB	03 Dec 2018 11:31:51	U	SMPL
J5770-14 - 1	OR-03-112918-A	-66	0.0383	-	7470A	PPB	03 Dec 2018 11:33:58	U	SMPL
J5770-16 - 1	OR-03-112918-B	-49	0.0428	-	7470A	PPB	03 Dec 2018 11:36:06	U	SMPL
J5771-08 - 1	EO-02-112918-A	-45	0.0438	-	7470A	PPB	03 Dec 2018 11:38:14	U	SMPL
J5771-10 - 1	EO-02-112918-B	-67	0.0380	-	7470A	PPB	03 Dec 2018 11:40:22	U	SMPL
J5771-12 - 1	EO-02-112918-C	-53	0.0417	-	7470A	PPB	03 Dec 2018 11:42:29	U	SMPL
J6140-01 - 1	PAINT-DEBRIS	-6	0.0542	-	7470A	PPB	03 Dec 2018 11:44:38	U	SMPL
J6140-02 - 1	PAINT-DEBRIS-WITH-PLASTIC	-24	0.0494	-	7470A	PPB	03 Dec 2018 11:46:46	U	SMPL
J6141-01 - 1	GD	3357	0.9465	-	7470A	PPB	03 Dec 2018 11:48:53	U	SMPL
CCV49 - 1	CCV49	18646	5.0032	-	7470A	PPB	03 Dec 2018 11:51:00	U	SMPL
CCB49 - 1	CCB49	-207	0.0008	-	7470A	PPB	03 Dec 2018 11:53:09	U	SMPL
PB115229BL - 1	PBW	-99	0.0295	-	7470A	PPB	03 Dec 2018 11:55:16	U	SMPL
PB115229BS - 1	LCSW	14337	3.8598	-	7470A	PPB	03 Dec 2018 11:57:24	U	SMPL
J6134-01 - 1	FB-1	-156	0.0144	-	7470A	PPB	03 Dec 2018 11:59:30	U	SMPL
J6134-02 - 1	MW-6	88	0.0791	-	7470A	PPB	03 Dec 2018 12:01:37	U	SMPL
J6134-03 - 1	MW-7	-37	0.0459	-	7470A	PPB	03 Dec 2018 12:03:45	U	SMPL
J6134-04 - 1	MW-8	-19	0.0507	-	7470A	PPB	03 Dec 2018 12:05:53	U	SMPL
J6134-05 - 1	MW-9	-17	0.0513	-	7470A	PPB	03 Dec 2018 12:08:01	U	SMPL
J6134-06 - 1	MW-11	-54	0.0414	-	7470A	PPB	03 Dec 2018 12:10:09	U	SMPL
J6134-07 - 1	DUP-1	-56	0.0409	-	7470A	PPB	03 Dec 2018 12:12:17	U	SMPL
J6134-07DUP - 1	DUP-1DUP	-63	0.0390	-	7470A	PPB	03 Dec 2018 12:14:24	U	SMPL
CCV50 - 1	CCV50	18749	5.0305	-	7470A	PPB	03 Dec 2018 12:16:32	U	SMPL
CCB50 - 1	CCB50	-143	0.0178	-	7470A	PPB	03 Dec 2018 12:18:39	U	SMPL
J6134-07MS - 1	DUP-1MS	14337	3.8598	-	7470A	PPB	03 Dec 2018 12:20:47	U	SMPL
J6134-07MSD - 1	DUP-1MSD	13983	3.7659	-	7470A	PPB	03 Dec 2018 12:22:54	U	SMPL
J6153-01 - 1	MH-F	-164	0.0123	-	7470A	PPB	03 Dec 2018 12:25:01	U	SMPL
J6153-02 - 1	MH-G	-131	0.0210	-	7470A	PPB	03 Dec 2018 12:27:08	U	SMPL
J6153-03 - 1	MH-J	-107	0.0274	-	7470A	PPB	03 Dec 2018 12:29:16	U	SMPL
J6153-04 - 1	MH-H	-96	0.0303	-	7470A	PPB	03 Dec 2018 12:31:23	U	SMPL
J6153-05 - 1	MH-9.41	-121	0.0237	-	7470A	PPB	03 Dec 2018 12:33:31	U	SMPL
PB115228TB - 1	PB115185TB	-48	0.0430	-	7470A	PPB	03 Dec 2018 12:35:40	U	SMPL
CCV51 - 1	CCV51	18968	5.0886	-	7470A	PPB	03 Dec 2018 12:37:48	U	SMPL
CCB51 - 1	CCB51	-130	0.0213	-	7470A	PPB	03 Dec 2018 12:39:56	U	SMPL
J5761-02LX5 - 1		-60	0.0398	-	7470A	PPB	03 Dec 2018 12:42:03	U	SMPL
J5761-02A - 1		15326	4.1223	-	7470A	PPB	03 Dec 2018 12:44:10	U	SMPL
J6134-07LX5 - 1		-111	0.0263	-	7470A	PPB	03 Dec 2018 12:46:18	U	SMPL
J6134-07A - 1		15581	4.1899	-	7470A	PPB	03 Dec 2018 12:48:25	U	SMPL
CCV52 - 1	CCV52	18556	4.9793	-	7470A	PPB	03 Dec 2018 12:50:32	U	SMPL
CCB52 - 1	CCB52	-157	0.0141	-	7470A	PPB	03 Dec 2018 12:52:39	U	SMPL