

LB99551


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

39771

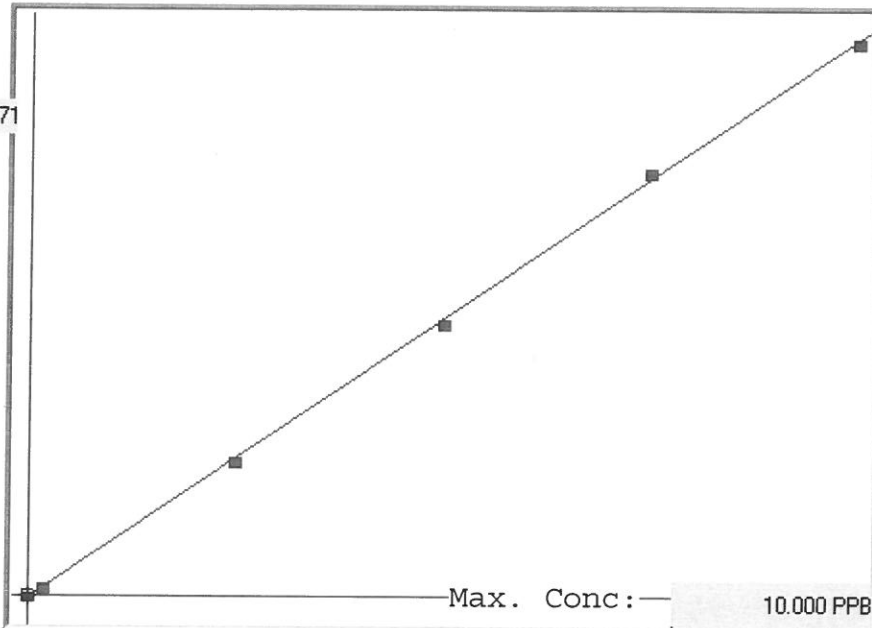

A= 0.0000e+000

B= 2.4909e-004

C= 4.0674e-002

Rho= 0.9998427

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.043	0.043	9	0.000	9				
0.2	0.200	0.195	-0.005	618	0.0 %	618				
2.5	2.500	2.452	-0.048	9681	0.0 %	9681				
5.0	5.000	4.940	-0.060	19670	0.0 %	19670				
7.5	7.500	7.623	0.123	30441	0.0 %	30441				
10.0	10.000	9.947	-0.053	39771	0.0 %	39771				

LB99551 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Dec 2018 08:25:44

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	9	-	0.0000	7470A	PPB	04 Dec 2018 08:35:53	S	Std
0.2 - 1	50.2	618	-	0.2000	7470A	PPB	04 Dec 2018 08:38:02	S	Std
2.5 - 1	52.5	9681	-	2.5000	7470A	PPB	04 Dec 2018 08:40:11	S	Std
5.0 - 1	55	19670	-	5.0000	7470A	PPB	04 Dec 2018 08:42:19	S	Std
7.5 - 1	57.5	30441	-	7.5000	7470A	PPB	04 Dec 2018 08:44:27	S	Std
10.0 - 1	510	39771	-	10.0000	7470A	PPB	04 Dec 2018 08:46:35	S	Std
ICV03 - 1	ICV03	15788	3.9732	-7470A	PPB	PPB	04 Dec 2018 08:49:23	U	SMPL
ICB03 - 1	ICB03	-71	0.0230	-7470A	PPB	PPB	04 Dec 2018 08:51:29	U	SMPL
CCV61 - 1	CCV61	19682	4.9432	-7470A	PPB	PPB	04 Dec 2018 08:53:36	U	SMPL
CCB61 - 1	CCB61	-64	0.0247	-7470A	PPB	PPB	04 Dec 2018 08:55:42	U	SMPL
CRA - 1	CRA	607	0.1919	-7470A	PPB	PPB	04 Dec 2018 08:57:49	U	SMPL
HighStd - 1	HighStd	38763	9.6960	-7470A	PPB	PPB	04 Dec 2018 08:59:56	U	SMPL
ChkStd - 1	ChkStd	27728	6.9473	-7470A	PPB	PPB	04 Dec 2018 09:02:02	U	SMPL
PB115273BL - 1	PBW	-157	0.0016	-7470A	PPB	PPB	04 Dec 2018 09:04:11	U	SMPL
PB115273BS - 1	LCSW	14207	3.5794	-7470A	PPB	PPB	04 Dec 2018 09:06:19	U	SMPL
J5764-22 - 1	JC-02-113018-A	-95	0.0170	-7470A	PPB	PPB	04 Dec 2018 09:08:27	U	SMPL
J5764-22DUP - 1	JC-02-113018-ADUP	-60	0.0257	-7470A	PPB	PPB	04 Dec 2018 09:10:36	U	SMPL
J5764-22MS - 1	JC-02-113018-AMS	13534	3.4118	-7470A	PPB	PPB	04 Dec 2018 09:12:44	U	SMPL
J5764-22MSD - 1	JC-02-113018-AMSD	12869	3.2462	-7470A	PPB	PPB	04 Dec 2018 09:14:52	U	SMPL
J5764-24 - 1	JC-02-113018-B	-112	0.0128	-7470A	PPB	PPB	04 Dec 2018 09:16:59	U	SMPL
CCV62 - 1	CCV62	19905	4.9987	-7470A	PPB	PPB	04 Dec 2018 09:19:06	U	SMPL
CCB62 - 1	CCB62	-64	0.0247	-7470A	PPB	PPB	04 Dec 2018 09:21:13	U	SMPL
J5764-26 - 1	JC-02-113018-C	-54	0.0272	-7470A	PPB	PPB	04 Dec 2018 09:23:20	U	SMPL
J5764-28 - 1	JC-02-113018-D	-48	0.0287	-7470A	PPB	PPB	04 Dec 2018 09:25:27	U	SMPL
J5764-30 - 1	JC-02-113018-E	-36	0.0317	-7470A	PPB	PPB	04 Dec 2018 09:27:34	U	SMPL
J5775-04 - 1	TR-04-113018	-58	0.0262	-7470A	PPB	PPB	04 Dec 2018 09:29:41	U	SMPL
J6149-01 - 1	ENGINE-WASH	-19	0.0359	-7470A	PPB	PPB	04 Dec 2018 09:31:49	U	SMPL
J6149-02 - 1	OWS-2	-37	0.0315	-7470A	PPB	PPB	04 Dec 2018 09:33:56	U	SMPL
J6149-03 - 1	BUS-WASH	-60	0.0257	-7470A	PPB	PPB	04 Dec 2018 09:36:05	U	SMPL
J6149-04 - 1	RECLAIMER-PIT	-42	0.0302	-7470A	PPB	PPB	04 Dec 2018 09:38:13	U	SMPL
J6150-01 - 1	WASTE-OIL-TOTES	-81	0.0205	-7470A	PPB	PPB	04 Dec 2018 09:40:21	U	SMPL
J6159-01 - 1	CB-1129-S-TCLP-GRID19	-28	0.0337	-7470A	PPB	PPB	04 Dec 2018 09:42:28	U	SMPL
CCV63 - 1	CCV63	19192	4.8211	-7470A	PPB	PPB	04 Dec 2018 09:44:35	U	SMPL
CCB63 - 1	CCB63	-65	0.0245	-7470A	PPB	PPB	04 Dec 2018 09:46:43	U	SMPL
J6159-02 - 1	CB-1129-S-TCLP-GRID26-1	-49	0.0285	-7470A	PPB	PPB	04 Dec 2018 09:48:50	U	SMPL
J6159-03 - 1	CB-1129-S-TCLP-GRID26-2	-42	0.0302	-7470A	PPB	PPB	04 Dec 2018 09:50:57	U	SMPL
J6159-04 - 1	CB-1129-S-TCLP-GRID27	-53	0.0275	-7470A	PPB	PPB	04 Dec 2018 09:53:04	U	SMPL
J6160-04 - 1	TEST-PIT	-47	0.0290	-7470A	PPB	PPB	04 Dec 2018 09:55:11	U	SMPL
PB115274BL - 1	PBW	-47	0.0290	-7470A	PPB	PPB	04 Dec 2018 09:57:19	U	SMPL
PB115274BS - 1	LCSW	14592	3.6753	-7470A	PPB	PPB	04 Dec 2018 09:59:26	U	SMPL
J6153-09 - 1	MH-F	-100	0.0158	-7470A	PPB	PPB	04 Dec 2018 10:01:35	U	SMPL
J6153-09DUP - 1	MH-FDUP	-36	0.0317	-7470A	PPB	PPB	04 Dec 2018 10:03:43	U	SMPL
J6153-09MS - 1	MH-FMS	14716	3.7062	-7470A	PPB	PPB	04 Dec 2018 10:05:52	U	SMPL
J6153-09MSD - 1	MH-FMSD	14559	3.6671	-7470A	PPB	PPB	04 Dec 2018 10:07:59	U	SMPL
CCV64 - 1	CCV64	19914	5.0010	-7470A	PPB	PPB	04 Dec 2018 10:10:06	U	SMPL
CCB64 - 1	CCB64	-77	0.0215	-7470A	PPB	PPB	04 Dec 2018 10:12:14	U	SMPL
J6153-10 - 1	MH-G	-40	0.0307	-7470A	PPB	PPB	04 Dec 2018 10:14:21	U	SMPL
J6153-11 - 1	MH-J	3	0.0414	-7470A	PPB	PPB	04 Dec 2018 10:16:29	U	SMPL
J6153-12 - 1	MH-H	22	0.0462	-7470A	PPB	PPB	04 Dec 2018 10:18:36	U	SMPL
J6153-13 - 1	MH-9.41	5	0.0419	-7470A	PPB	PPB	04 Dec 2018 10:20:43	U	SMPL
PB115275BL - 1	PBW	10	0.0432	-7470A	PPB	PPB	04 Dec 2018 10:22:50	U	SMPL
PB115275BS - 1	LCSW	14005	3.5291	-7470A	PPB	PPB	04 Dec 2018 10:24:58	U	SMPL
J6157-01 - 1	COMPOSITE-1-TOTAL	533	0.1734	-7470A	PPB	PPB	04 Dec 2018 10:27:06	U	SMPL
J6157-01DUP - 1	COMPOSITE-1-TOTALDUP	504	0.1662	-7470A	PPB	PPB	04 Dec 2018 10:29:14	U	SMPL
J6157-01MS - 1	COMPOSITE-1-TOTALMS	16146	4.0624	-7470A	PPB	PPB	04 Dec 2018 10:31:23	U	SMPL
J6157-01MSD - 1	COMPOSITE-1-TOTALMSD	16773	4.2186	-7470A	PPB	PPB	04 Dec 2018 10:33:30	U	SMPL
CCV65 - 1	CCV65	20091	5.0451	-7470A	PPB	PPB	04 Dec 2018 10:35:38	U	SMPL
CCB65 - 1	CCB65	-89	0.0185	-7470A	PPB	PPB	04 Dec 2018 10:37:45	U	SMPL
J6157-02 - 1	COMPOSITE-1-DISSOLVED	119	0.0703	-7470A	PPB	PPB	04 Dec 2018 10:39:52	U	SMPL
J6157-03 - 1	COMPOSITE-2-TOTAL	208	0.0925	-7470A	PPB	PPB	04 Dec 2018 10:42:00	U	SMPL
J6157-04 - 1	COMPOSITE-2-DISSOLVED	-68	0.0237	-7470A	PPB	PPB	04 Dec 2018 10:44:07	U	SMPL
J6157-05 - 1	COMPOSITE-3-TOTAL	129	0.0728	-7470A	PPB	PPB	04 Dec 2018 10:46:14	U	SMPL
J6157-06 - 1	COMPOSITE-3-DISSOLVED	-64	0.0247	-7470A	PPB	PPB	04 Dec 2018 10:48:21	U	SMPL
J6157-07 - 1	COMPOSITE-4-TOTAL	1117	0.3189	-7470A	PPB	PPB	04 Dec 2018 10:50:29	U	SMPL
J6157-08 - 1	COMPOSITE-4-DISSOLVED	57	0.0549	-7470A	PPB	PPB	04 Dec 2018 10:52:37	U	SMPL
J6157-09 - 1	COMPOSITE-5-TOTAL	1429	0.3966	-7470A	PPB	PPB	04 Dec 2018 10:54:45	U	SMPL
J6157-10 - 1	COMPOSITE-5-DISSOLVED	62	0.0561	-7470A	PPB	PPB	04 Dec 2018 10:56:54	U	SMPL
J6157-11 - 1	COMPOSITE-6-TOTAL	5086	1.3075	-7470A	PPB	PPB	04 Dec 2018 10:59:01	U	SMPL
CCV66 - 1	CCV66	19695	4.9464	-7470A	PPB	PPB	04 Dec 2018 11:01:09	U	SMPL
CCB66 - 1	CCB66	-125	0.0095	-7470A	PPB	PPB	04 Dec 2018 11:03:16	U	SMPL
J6157-12 - 1	COMPOSITE-6-DISSOLVED	585	0.1864	-7470A	PPB	PPB	04 Dec 2018 11:05:23	U	SMPL
J6185-01 - 1	MH-6	-186	-0.0057	-7470A	PPB	PPB	04 Dec 2018 11:07:31	U	SMPL
PB115273TB - 1	PB115230TB	-55	0.0270	-7470A	PPB	PPB	04 Dec 2018 11:09:38	U	SMPL
PB115274TB - 1	PB115238TB	-61	0.0255	-7470A	PPB	PPB	04 Dec 2018 11:11:46	U	SMPL
J5764-22LX5 - 1		-39	0.0310	-7470A	PPB	PPB	04 Dec 2018 11:13:53	U	SMPL
J5764-22A - 1		14267	3.5944	-7470A	PPB	PPB	04 Dec 2018 11:16:01	U	SMPL
J6153-09LX5 - 1		-84	0.0198	-7470A	PPB	PPB	04 Dec 2018 11:18:09	U	SMPL
J6153-09A - 1		15861	3.9914	-7470A	PPB	PPB	04 Dec 2018 11:20:18	U	SMPL
J6157-01LX5 - 1		15	0.0444	-7470A	PPB	PPB	04 Dec 2018 11:22:26	U	SMPL
J6157-01A - 1		17723	4.4552	-7470A	PPB	PPB	04 Dec 2018 11:24:34	U	SMPL
CCV67 - 1	CCV67	19131	4.8059	-7470A	PPB	PPB	04 Dec 2018 11:26:41	U	SMPL

LB99551 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Dec 2018 08:25:44

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB67 - 1	CCB67	-112	0.0128		7470A	PPB	04 Dec 2018 11:28:49	U	SMPL