

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/6/2018 15:20

Test: Total CN

Sample Id	^{ug/d} Result	Dil. 1 +	Response	Errors
ICV1	90.010	0.0	0.078	
ICB1	1.494	0.0	0.004	
CCV1	239.177	0.0	0.202	
CCB1	1.524	0.0	0.004	
PB115323BL	1.364	0.0	0.004	
PB115323BS	91.121	0.0	0.079	
MIDPB115323	242.044	0.0	0.204	
J6185-01	4.525	0.0	0.006	
J6185-01DUP	4.449	0.0	0.006	
J6185-01MS	38.463	0.0	0.035	
J6185-01MSD	38.008	0.0	0.034	
CCV2	254.571	0.0	0.215	
CCB2	1.270	0.0	0.004	

N	13
Mean	77.540
SD	100.7524
CV%	129.94

Aquakem v. 7.2AQ1

Results from time period:

Thu Dec 06 15:16:55 2018

Thu Dec 06 15:20:19 2018

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	1.4908	µg/l	12/6/2018 11:36:38	
5.OPPBCN	A	Total CN	P	5.9278	µg/l	12/6/2018 11:36:39	
10PPBCN	A	Total CN	P	11.3348	µg/l	12/6/2018 11:36:40	
50PPBCN	A	Total CN	P	50.7321	µg/l	12/6/2018 11:36:41	
100PPBCN	A	Total CN	P	96.5241	µg/l	12/6/2018 11:36:42	
250PPBCN	A	Total CN	P	246.8086	µg/l	12/6/2018 11:36:43	
500PPBCN	A	Total CN	P	502.1817	µg/l	12/6/2018 11:36:44	
ICV1	S	Total CN	P	90.0103	µg/l	12/6/2018 15:16:55	
ICB1	S	Total CN	P	1.4936	µg/l	12/6/2018 15:16:56	
CCV1	S	Total CN	P	239.1769	µg/l	12/6/2018 15:16:57	
CCB1	S	Total CN	P	1.5235	µg/l	12/6/2018 15:16:58	
PB115323BL	S	Total CN	P	1.3639	µg/l	12/6/2018 15:16:59	
PB115323BS	S	Total CN	P	91.1205	µg/l	12/6/2018 15:17:00	
MIDPB115323	S	Total CN	P	242.0438	µg/l	12/6/2018 15:17:01	
J6185-01	S	Total CN	P	4.5251	µg/l	12/6/2018 15:17:02	
J6185-01DUP	S	Total CN	P	4.449	µg/l	12/6/2018 15:17:03	
J6185-01MS	S	Total CN	P	38.4631	µg/l	12/6/2018 15:17:04	
J6185-01MSD	S	Total CN	P	38.0077	µg/l	12/6/2018 15:17:05	
CCV2	S	Total CN	P	254.5707	µg/l	12/6/2018 15:20:18	
CCB2	S	Total CN	P	1.2701	µg/l	12/6/2018 15:20:19	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/6/2018 15:03


Test Total CN

Accepted 12/6/2018 11:38

Factor 1201
Bias 0.003

Coeff. of det. 0.999842

Errors

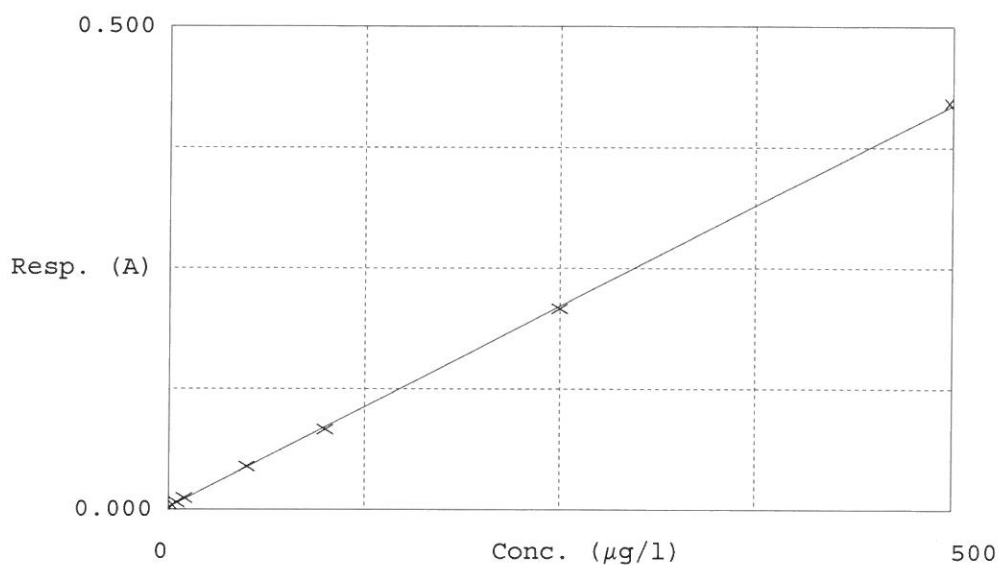

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	1.4908	0.0000	
2	5.0PPBCN	0.008	5.9278	5.0000	
3	10PPBCN	0.012	11.3348	10.0000	
4	50PPBCN	0.045	50.7321	50.0000	
5	100PPBCN	0.083	96.5241	100.0000	
6	250PPBCN	0.208	246.8086	250.0000	
7	500PPBCN	0.421	502.1817	500.0000	