

7470A


LB99638

INSTRUMENT ID: CV1

Linear

 μ Abs.:

37642

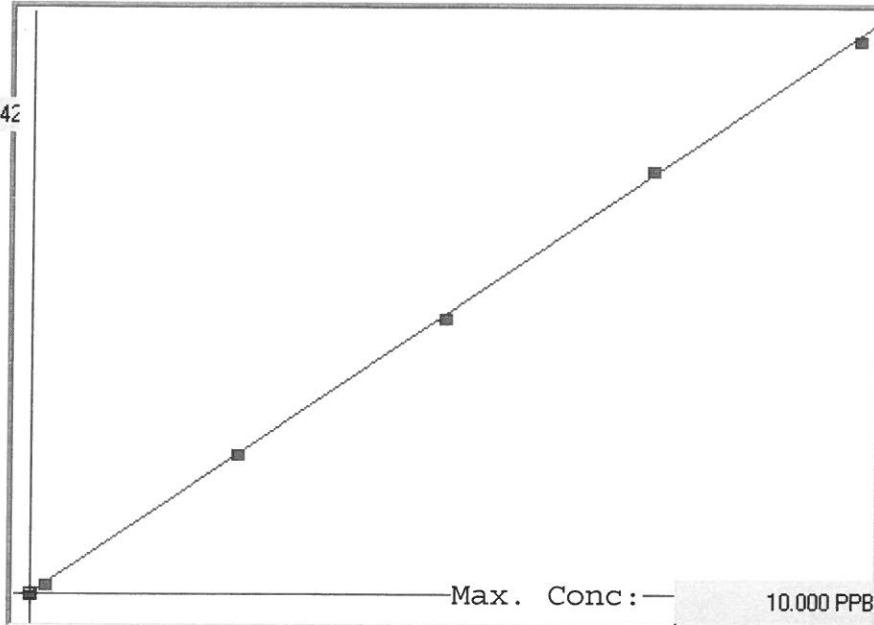

A= 0.0000e+000

B= 2.6377e-004

C= -2.5603e-003

Rho= 0.9998713

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.003	-0.003	0	0.000	0				
0.2	0.200	0.176	-0.024	677	0.0 %	677				
2.5	2.500	2.525	0.025	9584	0.0 %	9584				
5.0	5.000	4.962	-0.038	18820	0.0 %	18820				
7.5	7.500	7.613	0.113	28874	0.0 %	28874				
10.0	10.000	9.926	-0.074	37642	0.0 %	37642				

LB99638 INSTRUMENT : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Dec 2018 09:59:52

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	SD	0	-	0.00007470A	PPB	07 Dec 2018 10:02:52	S	Std
0.2 - 1	SD-2	677	-	0.20007470A	PPB	07 Dec 2018 10:05:00	S	Std
2.5 - 1	SD-5	9584	-	2.50007470A	PPB	07 Dec 2018 10:07:09	S	Std
5.0 - 1	SD-10	18820	-	5.00007470A	PPB	07 Dec 2018 10:09:18	S	Std
7.5 - 1	SD-15	28874	-	7.50007470A	PPB	07 Dec 2018 10:11:26	S	Std
10.0 - 1	SD-20	37642	-	10.00007470A	PPB	07 Dec 2018 10:13:34	S	Std
ICV10 - 1	ICV10	15249	4.0196	-7470A	PPB	07 Dec 2018 10:16:08	U	SMPL
ICB10 - 1	ICB10	-97	-0.0281	-7470A	PPB	07 Dec 2018 10:18:14	U	SMPL
CCV01 - 1	CCV01	18611	4.9064	-7470A	PPB	07 Dec 2018 10:20:20	U	SMPL
CCB01 - 1	CCB01	-95	-0.0276	-7470A	PPB	07 Dec 2018 10:22:27	U	SMPL
CRA - 1	CRA	649	0.1686	-7470A	PPB	07 Dec 2018 10:24:34	U	SMPL
HighStd - 1	HighStd	36621	9.6569	-7470A	PPB	07 Dec 2018 10:26:41	U	SMPL
ChkStd - 1	ChkStd	26520	6.9925	-7470A	PPB	07 Dec 2018 10:28:48	U	SMPL
PB115410BL - 1	PBW	-135	-0.0382	-7470A	PPB	07 Dec 2018 10:30:56	U	SMPL
PB115410BS - 1	LCSW	13562	3.5747	-7470A	PPB	07 Dec 2018 10:33:04	U	SMPL
J6195-02 - 1	OR-01-120518-A	-80	-0.0237	-7470A	PPB	07 Dec 2018 10:35:12	U	SMPL
J6195-02DUP - 1	OR-01-120518-ADUP	-29	-0.0102	-7470A	PPB	07 Dec 2018 10:37:20	U	SMPL
J6195-02MS - 1	OR-01-120518-AMS	12468	3.2861	-7470A	PPB	07 Dec 2018 10:39:29	U	SMPL
J6195-02MSD - 1	OR-01-120518-AMSD	12817	3.3781	-7470A	PPB	07 Dec 2018 10:41:38	U	SMPL
J6195-04 - 1	OR-01-120518-B	-80	-0.0237	-7470A	PPB	07 Dec 2018 10:43:44	U	SMPL
CCV02 - 1	CCV02	18580	4.8982	-7470A	PPB	07 Dec 2018 10:45:52	U	SMPL
CCB02 - 1	CCB02	-117	-0.0334	-7470A	PPB	07 Dec 2018 10:47:58	U	SMPL
J6199-02 - 1	SU-01-120518-A	-33	-0.0113	-7470A	PPB	07 Dec 2018 10:50:06	U	SMPL
J6199-04 - 1	SU-01-120518-B	-25	-0.0092	-7470A	PPB	07 Dec 2018 10:52:12	U	SMPL
J6234-03 - 1	VNJ-218	-15	-0.0065	-7470A	PPB	07 Dec 2018 10:54:19	U	SMPL
J6237-02 - 1	SAMPLE-2	-14	-0.0063	-7470A	PPB	07 Dec 2018 10:56:26	U	SMPL
J6243-01 - 1	OILY-DEBRIS	-23	-0.0086	-7470A	PPB	07 Dec 2018 10:58:34	U	SMPL
PB115411BL - 1	PBW	-8	-0.0047	-7470A	PPB	07 Dec 2018 11:00:42	U	SMPL
PB115411BS - 1	LCSW	12713	3.3507	-7470A	PPB	07 Dec 2018 11:02:50	U	SMPL
J6209-02 - 1	12.68	-63	-0.0192	-7470A	PPB	07 Dec 2018 11:04:58	U	SMPL
J6209-04 - 1	12.65	-14	-0.0063	-7470A	PPB	07 Dec 2018 11:07:06	U	SMPL
J6209-06 - 1	HMF-NORTH	-5	-0.0039	-7470A	PPB	07 Dec 2018 11:09:13	U	SMPL
CCV03 - 1	CCV03	18537	4.8869	-7470A	PPB	07 Dec 2018 11:11:20	U	SMPL
CCB03 - 1	CCB03	-94	-0.0274	-7470A	PPB	07 Dec 2018 11:13:27	U	SMPL
J6209-08 - 1	HMF-SOUTH	-14	-0.0063	-7470A	PPB	07 Dec 2018 11:15:34	U	SMPL
J6243-04 - 1	OILY-WATER-A	-14	-0.0063	-7470A	PPB	07 Dec 2018 11:17:41	U	SMPL
J6243-04DUP - 1	OILY-WATER-ADUP	-21	-0.0081	-7470A	PPB	07 Dec 2018 11:19:48	U	SMPL
J6243-04MS - 1	OILY-WATER-AMS	13159	3.4684	-7470A	PPB	07 Dec 2018 11:21:55	U	SMPL
J6243-04MSD - 1	OILY-WATER-AMSD	12874	3.3932	-7470A	PPB	07 Dec 2018 11:24:03	U	SMPL
J6243-07 - 1	OILY-WATER-B	-86	-0.0252	-7470A	PPB	07 Dec 2018 11:26:11	U	SMPL
PB115412BL - 1	PBW	-32	-0.0110	-7470A	PPB	07 Dec 2018 11:28:19	U	SMPL
PB115412BS - 1	LCSW	13841	3.6482	-7470A	PPB	07 Dec 2018 11:30:27	U	SMPL
J6214-33 - 1	TW-4	295	0.0753	-7470A	PPB	07 Dec 2018 11:37:17	U	SMPL
J6214-33DUP - 1	TW-4DUP	268	0.0681	-7470A	PPB	07 Dec 2018 11:39:23	U	SMPL
CCV04 - 1	CCV04	18693	4.9280	-7470A	PPB	07 Dec 2018 11:41:31	U	SMPL
CCB04 - 1	CCB04	-95	-0.0276	-7470A	PPB	07 Dec 2018 11:43:38	U	SMPL
J6214-33MS - 1	TW-4MS	15798	4.1644	-7470A	PPB	07 Dec 2018 11:45:45	U	SMPL
J6214-33MSD - 1	TW-4MSD	15589	4.1093	-7470A	PPB	07 Dec 2018 11:47:53	U	SMPL
J6214-36 - 1	TW-4	-173	-0.0482	-7470A	PPB	07 Dec 2018 11:50:00	U	SMPL
J6214-37 - 1	TW-10	2454	0.6447	-7470A	PPB	07 Dec 2018 11:52:08	U	SMPL
J6214-38 - 1	TW-10	-132	-0.0374	-7470A	PPB	07 Dec 2018 11:54:15	U	SMPL
J6214-39 - 1	TW-2	-97	-0.0281	-7470A	PPB	07 Dec 2018 11:56:23	U	SMPL
J6214-40 - 1	TW-2	-25	-0.0092	-7470A	PPB	07 Dec 2018 11:58:31	U	SMPL
J6243-03 - 1	OILY-WATER-A	-124	-0.0353	-7470A	PPB	07 Dec 2018 12:00:39	U	SMPL
J6243-06 - 1	OILY-WATER-B	-71	-0.0213	-7470A	PPB	07 Dec 2018 12:02:48	U	SMPL
J6250-02 - 1	BPS1-TT-MW304S-20181204	-113	-0.0324	-7470A	PPB	07 Dec 2018 12:04:55	U	SMPL
CCV05 - 1	CCV05	18345	4.8363	-7470A	PPB	07 Dec 2018 12:07:02	U	SMPL
CCB05 - 1	CCB05	-89	-0.0260	-7470A	PPB	07 Dec 2018 12:09:09	U	SMPL
J6250-03 - 1	BPS1-TT-MW304S-20181204	-113	-0.0324	-7470A	PPB	07 Dec 2018 12:11:17	U	SMPL
J6250-04 - 1	BPS1-TT-MW304I1-20181204	-109	-0.0313	-7470A	PPB	07 Dec 2018 12:13:24	U	SMPL
J6250-05 - 1	BPS1-TT-MW304I1-20181204	-116	-0.0332	-7470A	PPB	07 Dec 2018 12:15:32	U	SMPL
J6250-06 - 1	BPS1-TT-MW304I2-20181204	-103	-0.0297	-7470A	PPB	07 Dec 2018 12:17:39	U	SMPL
J6250-07 - 1	BPS1-TT-MW304I2-20181204	-121	-0.0345	-7470A	PPB	07 Dec 2018 12:19:46	U	SMPL
J6250-08 - 1	BPS1-TT-MW304D-20181204	-113	-0.0324	-7470A	PPB	07 Dec 2018 12:21:54	U	SMPL
J6250-09 - 1	BPS1-TT-MW304D-20181204	-116	-0.0332	-7470A	PPB	07 Dec 2018 12:24:02	U	SMPL
J6250-10 - 1	BPS1-TT-MW307S-20181204	-109	-0.0313	-7470A	PPB	07 Dec 2018 12:26:11	U	SMPL
J6250-11 - 1	BPS1-TT-MW307S-20181204	-109	-0.0313	-7470A	PPB	07 Dec 2018 12:28:20	U	SMPL
J6250-12 - 1	BPS1-TT-MW307I-20181204	-116	-0.0332	-7470A	PPB	07 Dec 2018 12:30:28	U	SMPL
CCV06 - 1	CCV06	18332	4.8328	-7470A	PPB	07 Dec 2018 12:32:35	U	SMPL
CCB06 - 1	CCB06	-85	-0.0250	-7470A	PPB	07 Dec 2018 12:34:43	U	SMPL
J6250-13 - 1	BPS1-TT-MW307I-20181204	-135	-0.0382	-7470A	PPB	07 Dec 2018 12:36:51	U	SMPL
J6250-14 - 1	BP-DUP01-20181204	-118	-0.0337	-7470A	PPB	07 Dec 2018 12:38:58	U	SMPL
J6250-15 - 1	BP-DUP01-20181204	-125	-0.0355	-7470A	PPB	07 Dec 2018 12:41:06	U	SMPL
PB115410TB - 1	PB115375TB	11	0.0003	-7470A	PPB	07 Dec 2018 12:43:14	U	SMPL
PB115411TB - 1	PB115377TB	-16	-0.0068	-7470A	PPB	07 Dec 2018 12:45:22	U	SMPL
CCV07 - 1	CCV07	18389	4.8479	-7470A	PPB	07 Dec 2018 12:47:30	U	SMPL
CCB07 - 1	CCB07	-90	-0.0263	-7470A	PPB	07 Dec 2018 12:49:38	U	SMPL
J6195-02LX5 - 1		-27	-0.0097	-7470A	PPB	07 Dec 2018 12:51:47	U	SMPL
J6195-02A - 1		15482	4.0811	-7470A	PPB	07 Dec 2018 12:53:55	U	SMPL
J6243-04LX5 - 1		-96	-0.0279	-7470A	PPB	07 Dec 2018 12:56:03	U	SMPL
J6243-04A - 1		15663	4.1288	-7470A	PPB	07 Dec 2018 12:58:11	U	SMPL
J6214-33LX5 - 1		-8	-0.0047	-7470A	PPB	07 Dec 2018 13:00:19	U	SMPL
J6214-33A - 1		15723	4.1447	-7470A	PPB	07 Dec 2018 13:02:26	U	SMPL
CCV08 - 1	CCV08	18522	4.8829	-7470A	PPB	07 Dec 2018 13:04:34	U	SMPL
CCB08 - 1	CCB08	-97	-0.0281	-7470A	PPB	07 Dec 2018 13:06:42	U	SMPL