


7470A

LB99690
INSTRUMENT ID:

Linear

 μ Abs.:

37254

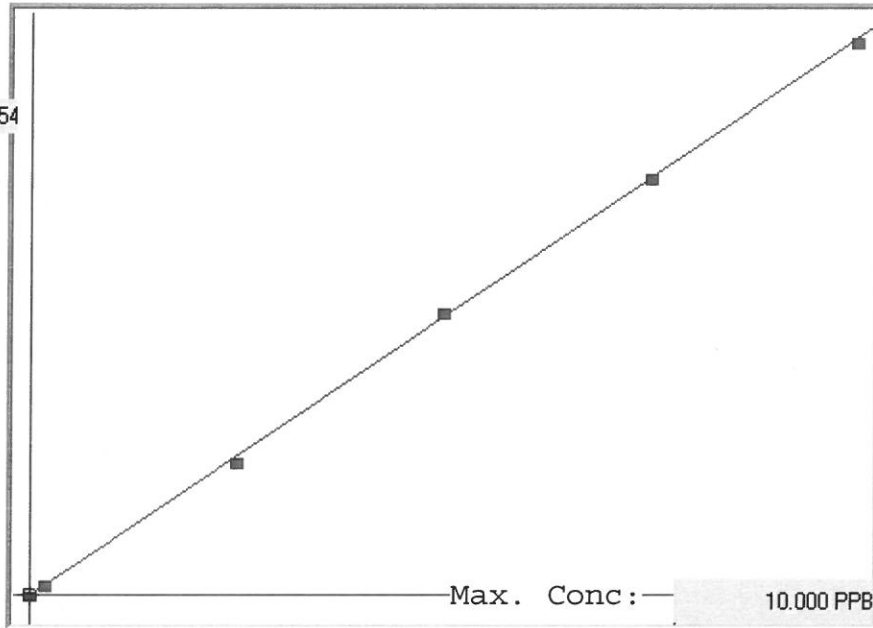

A= 0.0000e+000

B= 2.6661e-004

C= 1.9996e-002

Rho= 0.9998854

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.007	0.007	-49	0.000	-49				
0.2	0.200	0.195	-0.005	656	0.0 %	656				
2.5	2.500	2.426	-0.074	9023	0.0 %	9023				
5.0	5.000	5.103	0.103	19064	0.0 %	19064				
7.5	7.500	7.517	0.017	28121	0.0 %	28121				
10.0	10.000	9.952	-0.048	37254	0.0 %	37254				

LB99690 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Dec 2018 10:41:32

Sample ID	Extended ID	µ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-49	-	0.00007470A	PPB	10 Dec 2018 10:48:33	S	Std
0.2 - 1	50.2	656	-	0.20007470A	PPB	10 Dec 2018 10:50:42	S	Std
2.5 - 1	52.5	9023	-	2.50007470A	PPB	10 Dec 2018 10:52:51	S	Std
5.0 - 1	55	19064	-	5.00007470A	PPB	10 Dec 2018 10:54:59	S	Std
7.5 - 1	57.5	28121	-	7.50007470A	PPB	10 Dec 2018 10:57:07	S	Std
10.0 - 1	57.5	37254	-	10.00007470A	PPB	10 Dec 2018 10:59:15	S	Std
ICV13 - 1	ICV13	14450	3.8726	-7470A	PPB	10 Dec 2018 11:01:59	U	SMPL
ICB13 - 1	ICB13	-129	-0.0144	-7470A	PPB	10 Dec 2018 11:04:05	U	SMPL
CCV16 - 1	CCV16	18121	4.8513	-7470A	PPB	10 Dec 2018 11:06:12	U	SMPL
CCB16 - 1	CCB16	-134	-0.0157	-7470A	PPB	10 Dec 2018 11:08:18	U	SMPL
CRA - 1	CRA	640	0.1906	-7470A	PPB	10 Dec 2018 11:10:26	U	SMPL
HighStd - 1	HighStd	37625	10.0513	-7470A	PPB	10 Dec 2018 11:12:33	U	SMPL
ChkStd - 1	ChkStd	26690	7.1359	-7470A	PPB	10 Dec 2018 11:14:40	U	SMPL
PB115457BL - 1	PBW	-153	-0.0208	-7470A	PPB	10 Dec 2018 11:16:48	U	SMPL
PB115457BS - 1	LCSW	13374	3.5857	-7470A	PPB	10 Dec 2018 11:18:56	U	SMPL
J6259-02 - 1	BPS1-TT-MW306S-20181204	-188	-0.0301	-7470A	PPB	10 Dec 2018 11:21:04	U	SMPL
J6259-02DUP - 1	BPS1-TT-MW306S-20181204DUP	-103	-0.0075	-7470A	PPB	10 Dec 2018 11:23:12	U	SMPL
J6259-02MS - 1	BPS1-TT-MW306S-20181204MS	13819	3.7043	-7470A	PPB	10 Dec 2018 11:25:20	U	SMPL
J6259-02MSD - 1	BPS1-TT-MW306S-20181204MSD	13411	3.5955	-7470A	PPB	10 Dec 2018 11:27:29	U	SMPL
J6259-03 - 1	BPS1-TT-MW306S-20181204	-181	-0.0283	-7470A	PPB	10 Dec 2018 11:29:36	U	SMPL
CCV17 - 1	CCV17	18003	4.8198	-7470A	PPB	10 Dec 2018 11:31:43	U	SMPL
CCB17 - 1	CCB17	-136	-0.0163	-7470A	PPB	10 Dec 2018 11:33:49	U	SMPL
J6259-04 - 1	BPS1-TT-MW306I-20181205	-140	-0.0173	-7470A	PPB	10 Dec 2018 11:35:56	U	SMPL
J6259-05 - 1	BPS1-TT-MW306I-20181205	-137	-0.0165	-7470A	PPB	10 Dec 2018 11:38:02	U	SMPL
J6259-10 - 1	BPS1-TT-MW306D-20181205	-117	-0.0112	-7470A	PPB	10 Dec 2018 11:40:09	U	SMPL
J6259-11 - 1	BPS1-TT-MW306D-20181205	-130	-0.0147	-7470A	PPB	10 Dec 2018 11:42:16	U	SMPL
J6259-12 - 1	BPS1-TT-MW305S-20181205	-111	-0.0096	-7470A	PPB	10 Dec 2018 11:44:24	U	SMPL
J6259-13 - 1	BPS1-TT-MW305S-20181205	-121	-0.0123	-7470A	PPB	10 Dec 2018 11:46:33	U	SMPL
J6259-14 - 1	BPS1-TT-MW305I-20181205	-140	-0.0173	-7470A	PPB	10 Dec 2018 11:48:41	U	SMPL
J6259-15 - 1	BPS1-TT-MW305I-20181205	-127	-0.0139	-7470A	PPB	10 Dec 2018 11:50:49	U	SMPL
J6259-16 - 1	BPS1-TT-MW305D-20181205	-113	-0.0101	-7470A	PPB	10 Dec 2018 11:52:58	U	SMPL
J6259-17 - 1	BPS1-TT-MW305D-20181205	-124	-0.0131	-7470A	PPB	10 Dec 2018 11:55:06	U	SMPL
CCV18 - 1	CCV18	18099	4.8454	-7470A	PPB	10 Dec 2018 11:57:13	U	SMPL
CCB18 - 1	CCB18	-125	-0.0133	-7470A	PPB	10 Dec 2018 11:59:20	U	SMPL
J6259-18 - 1	BPS1-TT-MW302S-20181205	-118	-0.0115	-7470A	PPB	10 Dec 2018 12:01:27	U	SMPL
J6259-19 - 1	BPS1-TT-MW302S-20181205	-118	-0.0115	-7470A	PPB	10 Dec 2018 12:03:34	U	SMPL
J6259-20 - 1	BPS1-TT-MW302I1-20181205	-130	-0.0147	-7470A	PPB	10 Dec 2018 12:05:41	U	SMPL
J6259-21 - 1	BPS1-TT-MW302I1-20181205	-134	-0.0157	-7470A	PPB	10 Dec 2018 12:07:49	U	SMPL
J6259-22 - 1	BP-DUP02-20181205	-126	-0.0136	-7470A	PPB	10 Dec 2018 12:09:56	U	SMPL
J6259-23 - 1	BP-DUP02-20181205	-122	-0.0125	-7470A	PPB	10 Dec 2018 12:12:04	U	SMPL
J6259-24 - 1	BP-EB01-20181205	-56	0.0051	-7470A	PPB	10 Dec 2018 12:14:13	U	SMPL
J6259-25 - 1	BP-EB01-20181205	-63	0.0032	-7470A	PPB	10 Dec 2018 12:16:21	U	SMPL
PB115458BL - 1	PBW	-35	0.0107	-7470A	PPB	10 Dec 2018 12:18:30	U	SMPL
PB115458BS - 1	LCSW	13697	3.6718	-7470A	PPB	10 Dec 2018 12:20:37	U	SMPL
CCV19 - 1	CCV19	18113	4.8492	-7470A	PPB	10 Dec 2018 12:22:44	U	SMPL
CCB19 - 1	CCB19	-135	-0.0160	-7470A	PPB	10 Dec 2018 12:24:51	U	SMPL
J6218-01 - 1	MW-2R	-83	-0.0021	-7470A	PPB	10 Dec 2018 12:26:59	U	SMPL
J6218-02 - 1	MW-1	-3	0.0192	-7470A	PPB	10 Dec 2018 12:29:06	U	SMPL
J6218-03 - 1	SW-1	-156	-0.0216	-7470A	PPB	10 Dec 2018 12:31:13	U	SMPL
J6218-04 - 1	MW-6R	100	0.0467	-7470A	PPB	10 Dec 2018 12:33:21	U	SMPL
J6218-04DUP - 1	MW-6RDUP	108	0.0488	-7470A	PPB	10 Dec 2018 12:35:28	U	SMPL
J6218-04MS - 1	MW-6RMS	17987	4.8156	-7470A	PPB	10 Dec 2018 12:37:36	U	SMPL
J6218-04MSD - 1	MW-6RMSD	15653	4.1933	-7470A	PPB	10 Dec 2018 12:39:43	U	SMPL
J6218-05 - 1	MW-9R	141	0.0576	-7470A	PPB	10 Dec 2018 12:41:52	U	SMPL
J6235-01 - 1	MW-10	-82	-0.0019	-7470A	PPB	10 Dec 2018 12:44:01	U	SMPL
J6235-02 - 1	MW-8R	-68	0.0019	-7470A	PPB	10 Dec 2018 12:46:08	U	SMPL
CCV20 - 1	CCV20	18161	4.8620	-7470A	PPB	10 Dec 2018 12:48:15	U	SMPL
CCB20 - 1	CCB20	-147	-0.0192	-7470A	PPB	10 Dec 2018 12:50:22	U	SMPL
J6235-03 - 1	SW-3	-114	-0.0104	-7470A	PPB	10 Dec 2018 12:52:30	U	SMPL
J6235-04 - 1	MW-14	-95	-0.0053	-7470A	PPB	10 Dec 2018 12:54:37	U	SMPL
J6235-05 - 1	SW-2	-142	-0.0179	-7470A	PPB	10 Dec 2018 12:56:44	U	SMPL
J6235-06 - 1	DUP	-103	-0.0075	-7470A	PPB	10 Dec 2018 12:58:52	U	SMPL
J6269-03 - 1	OILY-WATER	333	0.1088	-7470A	PPB	10 Dec 2018 13:00:59	U	SMPL
J6259-02LX5 - 1		-68	0.0019	-7470A	PPB	10 Dec 2018 13:03:07	U	SMPL
J6259-02A - 1		15757	4.2210	-7470A	PPB	10 Dec 2018 13:05:15	U	SMPL
J6218-04LX5 - 1		-72	0.0008	-7470A	PPB	10 Dec 2018 13:07:23	U	SMPL
J6218-04A - 1		16642	4.4570	-7470A	PPB	10 Dec 2018 13:09:32	U	SMPL
CCV21 - 1	CCV21	18322	4.9049	-7470A	PPB	10 Dec 2018 13:11:40	U	SMPL
CCB21 - 1	CCB21	-136	-0.0163	-7470A	PPB	10 Dec 2018 13:13:47	U	SMPL