


245.1

LB 99732
INSTRUMENT ID: CV2

 μ Abs.:

34803

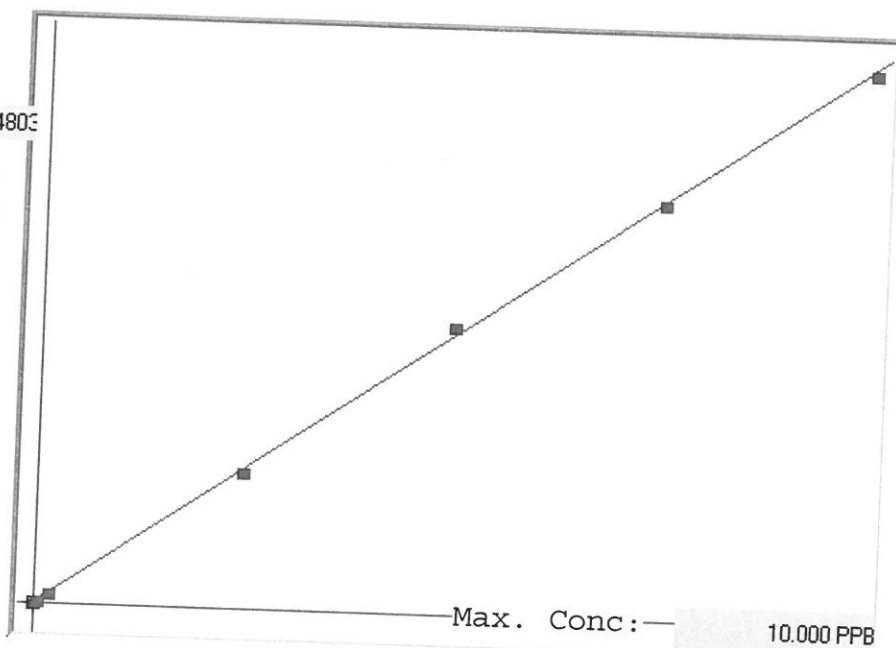

Linear

A= 0.0000e+000

B= 2.8571e-004

C= -1.4511e-002

Rho= 0.9997992

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.028	-0.028	-46	0.000	-46				
0.05	0.050	0.045	-0.005	209	0.0 %	209				
0.2	0.200	0.183	-0.017	693	0.0 %	693				
2.5	2.500	2.457	-0.043	8652	0.0 %	8652				
5.0	5.000	5.175	0.175	18164	0.0 %	18164				
7.5	7.500	7.487	-0.013	26257	0.0 %	26257				
10.0	10.000	9.929	-0.071	34803	0.0 %	34803				

Method: 245.1

Operator: Admin

LB99732 INSTRUMENT ID : CV1

Date of Analysis: 11 Dec 2018 14:22:31

Sample ID	Extended ID	μ Abs	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	-46	-	0.0000245.1	PPB	11 Dec 2018 14:29:04	S	Std
0.05 - 1	5005	209	-	0.0500245.1	PPB	11 Dec 2018 14:31:22	S	Std
0.2 - 1	502	693	-	0.2000245.1	PPB	11 Dec 2018 14:33:40	S	Std
2.5 - 1	505	8652	-	2.5000245.1	PPB	11 Dec 2018 14:35:57	S	Std
5.0 - 1	55	18164	-	5.0000245.1	PPB	11 Dec 2018 14:38:15	S	Std
7.5 - 1	575	26257	-	7.5000245.1	PPB	11 Dec 2018 14:40:31	S	Std
10.0 - 1	510	34803	-	10.0000245.1	PPB	11 Dec 2018 14:48:04	S	Std
ICV16 - 1	ICV16	13697	3.8989	-245.1	PPB	11 Dec 2018 14:50:48	U	SMPL
ICB16 - 1	ICB16	-148	-0.0568	-245.1	PPB	11 Dec 2018 14:53:04	U	SMPL
CCV39 - 1	CCV39	17870	5.0911	-245.1	PPB	11 Dec 2018 14:55:20	U	SMPL
CCB39 - 1	CCB39	-142	-0.0551	-245.1	PPB	11 Dec 2018 14:57:36	U	SMPL
CRA - 1	CRA	220	0.0483	-245.1	PPB	11 Dec 2018 14:59:53	U	SMPL
HighStd - 1	HighStd	34892	9.9545	-245.1	PPB	11 Dec 2018 15:02:09	U	SMPL
ChkStd - 1	ChkStd	24718	7.0477	-245.1	PPB	11 Dec 2018 15:04:25	U	SMPL
PB115523BL - 1	PBW	-84	-0.0385	-245.1	PPB	11 Dec 2018 15:06:43	U	SMPL
PB115523BS - 1	LCSW	12651	3.6000	-245.1	PPB	11 Dec 2018 15:09:02	U	SMPL
J6214-55 - 1	TW-2	3319	0.9338	-245.1	PPB	11 Dec 2018 15:11:20	U	SMPL
J6214-55DUP - 1	TW-2DUP	3466	0.9758	-245.1	PPB	11 Dec 2018 15:13:38	U	SMPL
J6214-55MS - 1	TW-2MS	18529	5.2794	-245.1	PPB	11 Dec 2018 15:15:56	U	SMPL
J6214-55MSD - 1	TW-2MSD	18509	5.2737	-245.1	PPB	11 Dec 2018 15:18:13	U	SMPL
J6257-02 - 1	GRAB	0	-0.0145	-245.1	PPB	11 Dec 2018 15:20:29	U	SMPL
CCV40 - 1	CCV40	17652	5.0288	-245.1	PPB	11 Dec 2018 15:22:45	U	SMPL
CCB40 - 1	CCB40	-125	-0.0502	-245.1	PPB	11 Dec 2018 15:25:01	U	SMPL
J6318-01 - 1	WEST-8TH-BOX-COVER-TEST-PIT	5562	1.5746	-245.1	PPB	11 Dec 2018 15:27:17	U	SMPL
J6326-01 - 1	120618-JETT-F-D-B	-14	-0.0185	-245.1	PPB	11 Dec 2018 15:29:33	U	SMPL
J6326-02 - 1	120618-JETT-F-D-S	-8	-0.0168	-245.1	PPB	11 Dec 2018 15:31:50	U	SMPL
J6326-03 - 1	120618-JETT-F-U-B	-25	-0.0217	-245.1	PPB	11 Dec 2018 15:34:06	U	SMPL
J6326-04 - 1	120618-JETT-F-U-S	-6	-0.0162	-245.1	PPB	11 Dec 2018 15:36:23	U	SMPL
J6326-05 - 1	120618-DBRI-F-D-B	-16	-0.0191	-245.1	PPB	11 Dec 2018 15:38:40	U	SMPL
J6326-06 - 1	120618-DBRI-F-D-S	-21	-0.0205	-245.1	PPB	11 Dec 2018 15:40:58	U	SMPL
J6326-07 - 1	120618-DBRI-F-U-B	-14	-0.0185	-245.1	PPB	11 Dec 2018 15:43:15	U	SMPL
J6326-08 - 1	120618-DBRI-F-U-S	-17	-0.0194	-245.1	PPB	11 Dec 2018 15:45:33	U	SMPL
J6326-09 - 1	120618-TIPC-E-D-M	-8	-0.0168	-245.1	PPB	11 Dec 2018 15:47:50	U	SMPL
CCV41 - 1	CCV41	17903	5.1005	-245.1	PPB	11 Dec 2018 15:50:06	U	SMPL
CCB41 - 1	CCB41	-116	-0.0477	-245.1	PPB	11 Dec 2018 15:52:23	U	SMPL
J6326-10 - 1	120618-TIPC-E-U-M	-23	-0.0211	-245.1	PPB	11 Dec 2018 15:54:39	U	SMPL
J6328-01 - 1	120718-JETT-F-D-B	-5	-0.0159	-245.1	PPB	11 Dec 2018 15:56:55	U	SMPL
J6328-02 - 1	120718-JETT-F-D-S	-13	-0.0182	-245.1	PPB	11 Dec 2018 15:59:12	U	SMPL
J6328-03 - 1	120718-JETT-F-U-B	-4	-0.0157	-245.1	PPB	11 Dec 2018 16:01:28	U	SMPL
J6328-04 - 1	120718-JETT-F-U-S	2	-0.0139	-245.1	PPB	11 Dec 2018 16:03:45	U	SMPL
J6214-55LX5 - 1		502	0.1289	-245.1	PPB	11 Dec 2018 16:06:02	U	SMPL
J6214-55A - 1		20401	5.8142	-245.1	PPB	11 Dec 2018 16:08:20	U	SMPL
CCV42 - 1	CCV42	17696	5.0414	-245.1	PPB	11 Dec 2018 16:10:38	U	SMPL
CCB42 - 1	CCB42	-114	-0.0471	-245.1	PPB	11 Dec 2018 16:12:56	U	SMPL