

=====

Test results

Aquakem 7.2AQ1

21399815
Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : as

12/14/2018 9:55

Test: Total CN

ug/l

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.986	0.0	0.088	
ICB1	0.548	0.0	0.004	
CCV1	237.879	0.0	0.217	
CCB1	0.299	0.0	0.004	
PB115658BL	0.450	0.0	0.004	
PB115658BS	95.458	0.0	0.089	
MIDPB115658	239.302	0.0	0.219	
J6223-01	0.652	0.0	0.004	
J6223-01DUP	0.581	0.0	0.004	
J6223-01MS	42.337	0.0	0.042	
J6223-01MSD	41.270	0.0	0.041	
CCV2	253.022	0.0	0.231	
CCB2	0.490	0.0	0.004	

N	13
Mean	77.406
SD	100.5913
CV%	129.95

Aquakem v. 7.2AQ1

Results from time period:

Fri Dec 14 09:52:04 2018

Fri Dec 14 09:55:28 2018

✓ AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.0268	µg/l	12/14/2018 7:35:33	
5.0PPBCN	A	Total CN	P	4.5915	µg/l	12/14/2018 7:35:34	
10PPBCN	A	Total CN	P	9.666	µg/l	12/14/2018 7:35:35	
50PPBCN	A	Total CN	P	49.5859	µg/l	12/14/2018 7:35:36	
100PPBCN	A	Total CN	P	99.7042	µg/l	12/14/2018 7:35:37	
250PPBCN	A	Total CN	P	252.6286	µg/l	12/14/2018 7:35:38	
500PPBCN	A	Total CN	P	498.7971	µg/l	12/14/2018 7:35:39	
ICV1	S	Total CN	P	93.9859	µg/l	12/14/2018 9:52:04	
ICB1	S	Total CN	P	0.548	µg/l	12/14/2018 9:52:05	
CCV1	S	Total CN	P	237.879	µg/l	12/14/2018 9:52:06	
CCB1	S	Total CN	P	0.2987	µg/l	12/14/2018 9:52:07	
PB115658BL	S	Total CN	P	0.4503	µg/l	12/14/2018 9:52:08	
PB115658BS	S	Total CN	P	95.4582	µg/l	12/14/2018 9:52:09	
MIDPB115658	S	Total CN	P	239.3022	µg/l	12/14/2018 9:52:10	
J6223-01	S	Total CN	P	0.6524	µg/l	12/14/2018 9:52:11	
J6223-01DUP	S	Total CN	P	0.5814	µg/l	12/14/2018 9:52:12	
J6223-01MS	S	Total CN	P	42.3368	µg/l	12/14/2018 9:52:13	
J6223-01MSD	S	Total CN	P	41.2698	µg/l	12/14/2018 9:52:14	
CCV2	S	Total CN	P	253.0219	µg/l	12/14/2018 9:55:27	
CCB2	S	Total CN	P	0.4902	µg/l	12/14/2018 9:55:28	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/14/2018 7:36


Test Total CN

Accepted 12/14/2018 7:36

Factor 1112
Bias 0.003

Coeff. of det. 0.999957

Errors

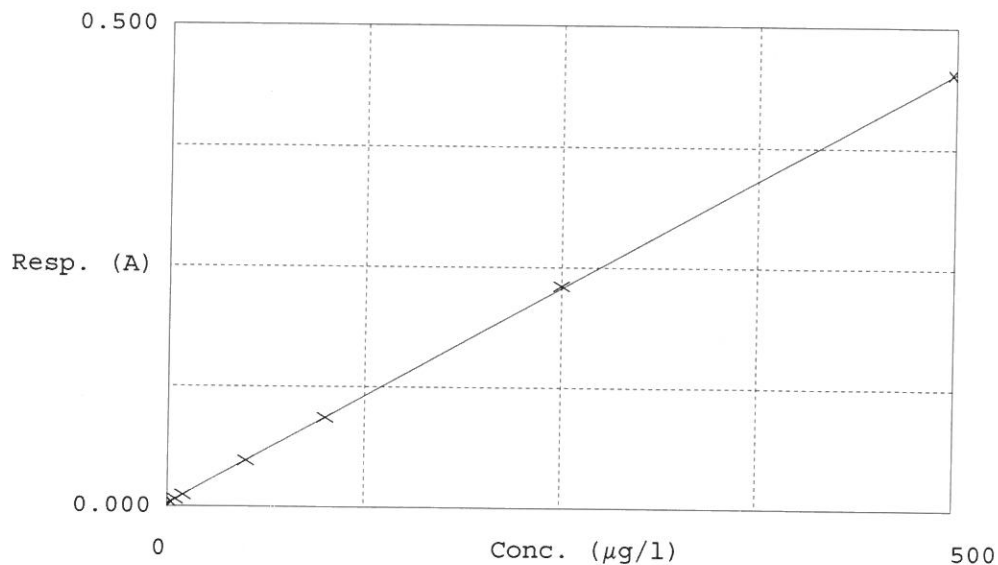

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.0268	0.0000	
2	5.0PPBCN	0.008	4.5915	5.0000	
3	10PPBCN	0.012	9.6660	10.0000	
4	50PPBCN	0.048	49.5859	50.0000	
5	100PPBCN	0.093	99.7042	100.0000	
6	250PPBCN	0.231	252.6286	250.0000	
7	500PPBCN	0.452	498.7971	500.0000	