

LB99816


245.1

INSTRUMENT ID: CV3

Linear

 μ Abs.:

33728

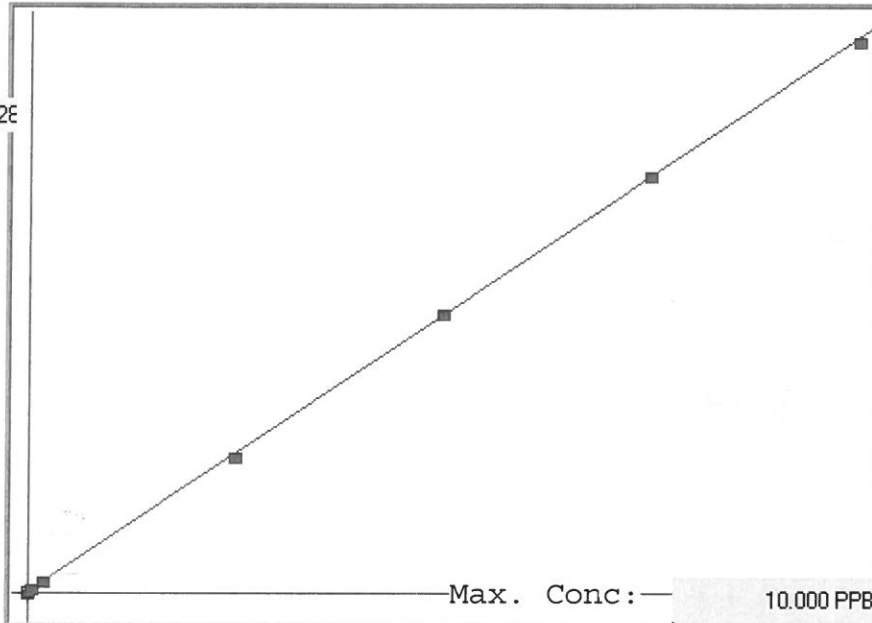

A= 0.0000e+000

B= 2.9569e-004

C= -1.3361e-002

Rho= 0.9999632

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.014	-0.014	-2	0.000	-2				
0.05	0.050	0.062	0.012	256	0.0 %	256				
0.2	0.200	0.204	0.004	735	0.0 %	735				
2.5	2.500	2.457	-0.043	8355	0.0 %	8355				
5.0	5.000	5.042	0.042	17096	0.0 %	17096				
7.5	7.500	7.539	0.039	25542	0.0 %	25542				
10.0	10.000	9.960	-0.040	33728	0.0 %	33728				

LB99816 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 14 Dec 2018 10:21:00

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-2	-	0.0000	245.1	PPB	14 Dec 2018 10:25:09	S	Std
0.05 - 1	50-05	256	-	0.0500	245.1	PPB	14 Dec 2018 10:27:27	S	Std
0.2 - 1	50-2	735	-	0.2000	245.1	PPB	14 Dec 2018 10:29:44	S	Std
2.5 - 1	50-5	8355	-	2.5000	245.1	PPB	14 Dec 2018 10:32:02	S	Std
5.0 - 1	55	17096	-	5.0000	245.1	PPB	14 Dec 2018 10:37:01	S	Std
7.5 - 1	57.5	25542	-	7.5000	245.1	PPB	14 Dec 2018 10:44:45	S	Std
10.0 - 1	SID	33728	-	10.0000	245.1	PPB	14 Dec 2018 10:47:02	S	Std
ICV23 - 1	ICV23	13101	3.8605	-245.1		PPB	14 Dec 2018 10:52:36	U	SMPL
ICB23 - 1	ICB23	-79	-0.0367	-245.1		PPB	14 Dec 2018 10:54:51	U	SMPL
CCV89 - 1	CCV89	16984	5.0086	-245.1		PPB	14 Dec 2018 10:57:07	U	SMPL
CCB89 - 1	CCB89	-97	-0.0420	-245.1		PPB	14 Dec 2018 10:59:23	U	SMPL
CRA - 1	CRA	250	0.0606	-245.1		PPB	14 Dec 2018 11:01:39	U	SMPL
HighStd - 1	HighStd	33864	9.9999	-245.1		PPB	14 Dec 2018 11:03:55	U	SMPL
ChkStd - 1	ChkStd	23434	6.9158	-245.1		PPB	14 Dec 2018 11:06:10	U	SMPL
PB115612BL - 1	PBW	-118	-0.0483	-245.1		PPB	14 Dec 2018 11:08:28	U	SMPL
PB115612BS - 1	LCSW	14861	4.3809	-245.1		PPB	14 Dec 2018 11:10:46	U	SMPL
J6223-02 - 1	EFFLUENT-METALS	532	0.1439	-245.1		PPB	14 Dec 2018 11:13:03	U	SMPL
J6341-03 - 1	121018-JETT-F-D-B	-95	-0.0415	-245.1		PPB	14 Dec 2018 11:15:21	U	SMPL
J6341-04 - 1	121018-JETT-F-D-S	-53	-0.0290	-245.1		PPB	14 Dec 2018 11:17:39	U	SMPL
J6341-05 - 1	121018-JETT-F-U-B	-11	-0.0166	-245.1		PPB	14 Dec 2018 11:19:57	U	SMPL
J6341-06 - 1	121018-JETT-F-U-S	-46	-0.0270	-245.1		PPB	14 Dec 2018 11:22:12	U	SMPL
CCV90 - 1	CCV90	17028	5.0216	-245.1		PPB	14 Dec 2018 11:24:29	U	SMPL
CCB90 - 1	CCB90	-103	-0.0438	-245.1		PPB	14 Dec 2018 11:26:44	U	SMPL
J6347-14 - 1	P001-TW001-01	-75	-0.0355	-245.1		PPB	14 Dec 2018 11:29:01	U	SMPL
J6347-14DUP - 1	P001-TW001-01DUP	-57	-0.0302	-245.1		PPB	14 Dec 2018 11:31:17	U	SMPL
J6347-15 - 1	J6347-14MS	13318	3.9246	-245.1		PPB	14 Dec 2018 11:33:33	U	SMPL
J6347-16 - 1	J6347-14MSD	12918	3.8064	-245.1		PPB	14 Dec 2018 11:35:50	U	SMPL
J6347-17 - 1	P001-TW001-02	-139	-0.0545	-245.1		PPB	14 Dec 2018 11:38:07	U	SMPL
J6347-18 - 1	P001-TW002-01	-86	-0.0388	-245.1		PPB	14 Dec 2018 11:40:24	U	SMPL
J6363-01 - 1	121118-JETT-F-D-B	-52	-0.0287	-245.1		PPB	14 Dec 2018 11:42:41	U	SMPL
J6363-02 - 1	121118-JETT-F-D-S	-45	-0.0267	-245.1		PPB	14 Dec 2018 11:44:58	U	SMPL
J6363-03 - 1	121118-JETT-F-U-B	-43	-0.0261	-245.1		PPB	14 Dec 2018 11:47:17	U	SMPL
J6363-04 - 1	121118-JETT-F-U-S	-28	-0.0216	-245.1		PPB	14 Dec 2018 11:49:33	U	SMPL
CCV91 - 1	CCV91	17085	5.0385	-245.1		PPB	14 Dec 2018 11:51:50	U	SMPL
CCB91 - 1	CCB91	-117	-0.0480	-245.1		PPB	14 Dec 2018 11:54:06	U	SMPL
J6385-01 - 1	121218-JETT-F-D-B	-51	-0.0284	-245.1		PPB	14 Dec 2018 11:56:23	U	SMPL
J6385-02 - 1	121218-JETT-F-D-S	-41	-0.0255	-245.1		PPB	14 Dec 2018 11:58:39	U	SMPL
J6385-03 - 1	121218-JETT-F-U-B	-13	-0.0172	-245.1		PPB	14 Dec 2018 12:00:55	U	SMPL
J6385-04 - 1	121218-JETT-F-U-S	-54	-0.0293	-245.1		PPB	14 Dec 2018 12:03:12	U	SMPL
J6347-14LX5 - 1		-15	-0.0178	-245.1		PPB	14 Dec 2018 12:05:29	U	SMPL
J6347-14A - 1		14305	4.2165	-245.1		PPB	14 Dec 2018 12:07:46	U	SMPL
CCV92 - 1	CCV92	16890	4.9808	-245.1		PPB	14 Dec 2018 12:10:03	U	SMPL
CCB92 - 1	CCB92	-102	-0.0435	-245.1		PPB	14 Dec 2018 12:12:21	U	SMPL