

2B100272

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

1/11/2019 14:57

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.926	0.0	0.086	
ICB1	-0.651	0.0	0.004	
CCV1	240.984	0.0	0.211	
CCB1	-0.544	0.0	0.004	
PB116331BL	-0.723	0.0	0.004	
PB116331BS	96.720	0.0	0.088	
MIDPB116331	242.672	0.0	0.213	
K1103-01	3.603	0.0	0.008	
K1103-01DUP	3.544	0.0	0.008	
K1103-01MS	35.391	0.0	0.035	
K1103-01MSD	35.245	0.0	0.035	
CCV2	258.080	0.0	0.226	
CCB2	-1.109	0.0	0.004	

N	13
Mean	77.549
SD	102.5819
CV%	132.28

Aquakem v. 7.2AQ1

✓A

Results from time period:

Fri Jan 11 14:54:08 2019

Fri Jan 11 14:57:32 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.3691	µg/l	1/11/2019 11:55:37	
5.0PPBCN	A	Total CN	P	4.0239	µg/l	1/11/2019 11:55:38	
10PPBCN	A	Total CN	P	9.0988	µg/l	1/11/2019 11:55:39	
50PPBCN	A	Total CN	P	49.9566	µg/l	1/11/2019 11:55:40	
100PPBCN	A	Total CN	P	100.7697	µg/l	1/11/2019 11:55:41	
250PPBCN	A	Total CN	P	253.2839	µg/l	1/11/2019 11:55:42	
500PPBCN	A	Total CN	P	498.2362	µg/l	1/11/2019 11:55:43	
ICV1	S	Total CN	P	94.9264	µg/l	1/11/2019 14:54:08	
ICB1	S	Total CN	P	-0.6508	µg/l	1/11/2019 14:54:09	
CCV1	S	Total CN	P	240.9839	µg/l	1/11/2019 14:54:10	
CCB1	S	Total CN	P	-0.5436	µg/l	1/11/2019 14:54:11	
PB116331BL	S	Total CN	P	-0.7228	µg/l	1/11/2019 14:54:12	
PB116331BS	S	Total CN	P	96.7201	µg/l	1/11/2019 14:54:13	
MIDPB116331	S	Total CN	P	242.6724	µg/l	1/11/2019 14:54:14	
K1103-01	S	Total CN	P	3.6027	µg/l	1/11/2019 14:54:15	
K1103-01DUP	S	Total CN	P	3.5439	µg/l	1/11/2019 14:54:16	
K1103-01MS	S	Total CN	P	35.3907	µg/l	1/11/2019 14:54:17	
K1103-01MSD	S	Total CN	P	35.2453	µg/l	1/11/2019 14:54:18	
CCV2	S	Total CN	P	258.08	µg/l	1/11/2019 14:57:31	
CCB2	S	Total CN	P	-1.1085	µg/l	1/11/2019 14:57:32	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

1/11/2019 11:58


Test Total CN

Accepted 1/11/2019 11:58

Factor 1165
Bias 0.005

Coeff. of det. 0.999920

Errors

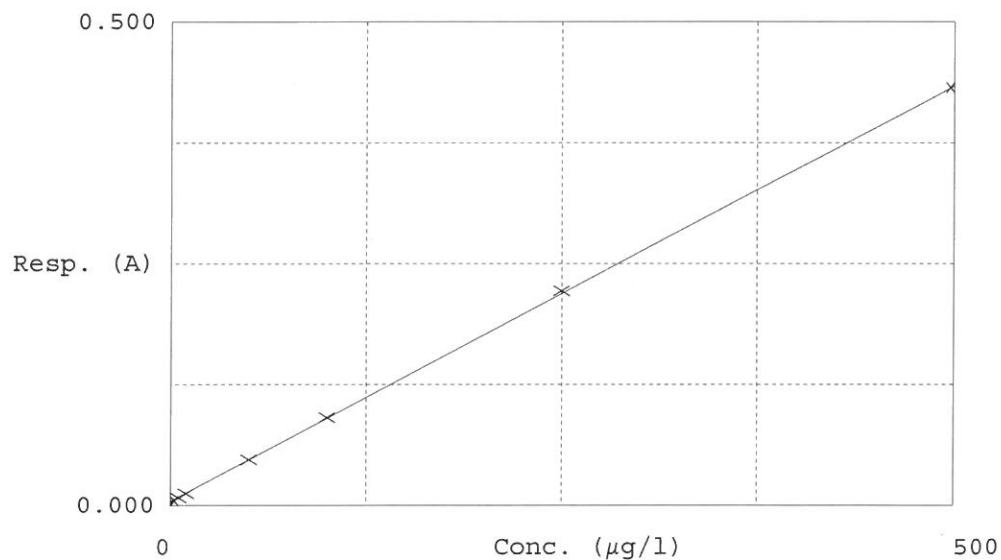

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.3691	0.0000	
2	5.0PPBCN	0.008	4.0239	5.0000	
3	10PPBCN	0.012	9.0988	10.0000	
4	50PPBCN	0.047	49.9566	50.0000	
5	100PPBCN	0.091	100.7697	100.0000	
6	250PPBCN	0.222	253.2839	250.0000	
7	500PPBCN	0.432	498.2362	500.0000	