

Clear table


IC-2 300'0
01-18-19 AD

ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-01-14	1/14/19 9:36		AK/AP
STD2	0.1430	0.1980	0.2420	0.7050	0.1810	-0.2590	1.2690	2019-01-14	1/14/19 10:07		AK/AP
STD3	0.4260	0.6270	0.6120	2.0280	0.5080	1.0820	3.1070	2019-01-14	1/14/19 10:38		AK/AP
STD4	0.8320	1.2110	1.1910	4.0420	1.0110	2.4220	5.9540	2019-01-14	1/14/19 11:10		AK/AP
STD5	1.8260	2.8340	2.8170	9.4550	2.3550	5.1140	13.9270	2019-01-14	1/14/19 11:41		AK/AP
STD6	4.1030	6.1270	6.1170	20.4380	5.1130	10.2710	30.6230	2019-01-14	1/14/19 12:13		AK/AP
STD7	4.9700	7.4540	7.4710	24.8320	6.2080	12.1190	37.3700	2019-01-14	1/14/19 12:44		AK/AP
ICV	1.9780	2.9140	2.8940	9.8180	2.4320	5.3910	14.3180	2019-01-14	1/14/19 14:18		AK/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-01-14	1/14/19 14:54		AK/AP
CCV	1.8810	2.9170	2.9070	9.7800	2.4240	4.7300	14.2890	2019-01-16	1/16/19 7:52		AK/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-01-16	1/16/19 8:34		AK/AP
LB100364BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-01-16	1/16/19 9:05		AK/AP
LB100364BSW	1.9420	2.9790	2.9150	9.8420	2.4460	5.3200	14.3550	2019-01-16	1/16/19 9:37		AK/AP
K1166-01	0.2790	36.3670	0.0000	0.0000	3.7230	1.8690	21.6190	2019-01-16	1/16/19 16:29		AK/AP
K1166-02	0.1950	16.5850	0.0000	0.0000	0.2640	0.0000	7.5130	2019-01-16	1/16/19 17:01		AK/AP
K1166-01DUP	0.2630	36.4610	0.0000	0.0000	3.7330	1.8840	21.6940	2019-01-16	1/16/19 17:32		AK/AP
K1166-01MS	2.2660	36.4830	2.8440	9.5210	5.8660	8.0700	34.2240	2019-01-16	1/16/19 18:04		AK/AP
K1166-01MSD	2.2440	36.5030	3.0420	10.1250	6.0060	8.4370	35.0760	2019-01-16	1/16/19 18:35		AK/AP
CCV	2.0470	2.9560	2.9250	9.9440	2.4760	5.4750	14.4050	2019-01-16	1/16/19 19:07		AK/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-01-16	1/16/19 19:38		AK/AP

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-011419.mtw
 Equation: $Q = 0.016869 \cdot A + 1.47281$
 RSD: 5.202 %
 Correlation coefficient: 0.998895

IC-2 cal
 01-14-19 AR

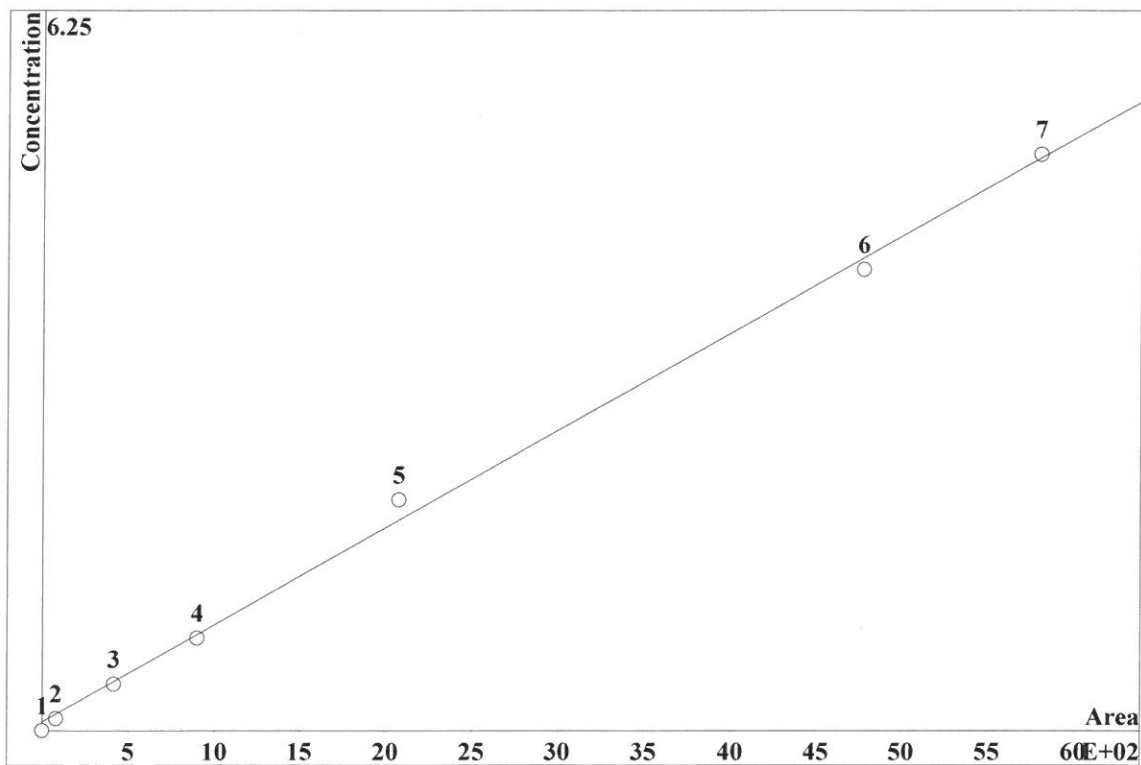


K3 = 0 K2 = 0 K1 = 0.016869 K0 = 1.47281
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.546	82.42	0.1	20	5.166		
3	17.91	417.7	0.4	20	5.166		
4	37.75	899.2	0.8	20	5.166		
5	89.09	2077	2	20	5.166		
6	211.2	4777	4	20	5.166		
7	247.7	5805	5	20	5.166		

1.□

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-011419.mtw
 Equation: $Q = 0.0269857 \cdot A + 1.34507$
 RSD: 3.592 %
 Correlation coefficient: 0.999473

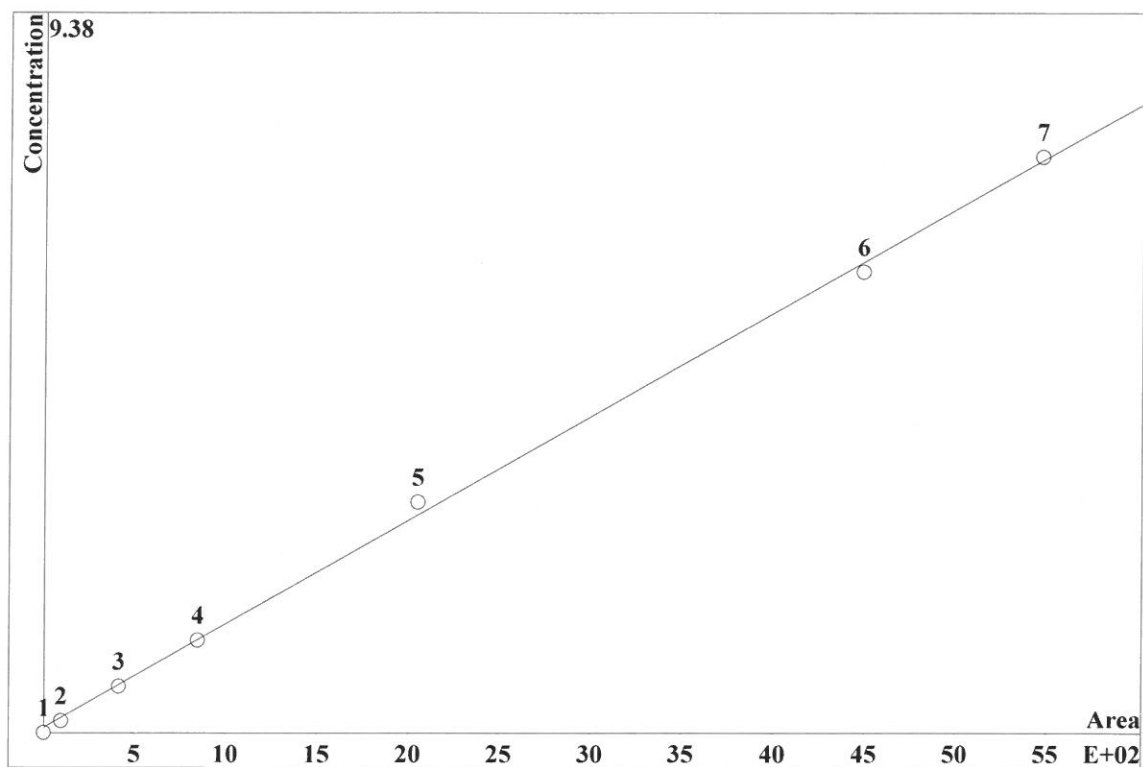


K3 = 0 K2 = 0 K1 = 0.0269857 K0 = 1.34507
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.778	96.57	0.15	20	9.024		
3	22.21	414.9	0.6	20	9.024		
4	46.78	847.7	1.2	20	9.024		
5	113.4	2051	3	20	9.024		
6	253.9	4491	6	20	9.024		
7	308.2	5474	7.5	20	9.024		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-011419.mtw
 Equation: $Q = 0.0114575 \cdot A + 2.72962$
 RSD: 3.869 %
 Correlation coefficient: 0.999389

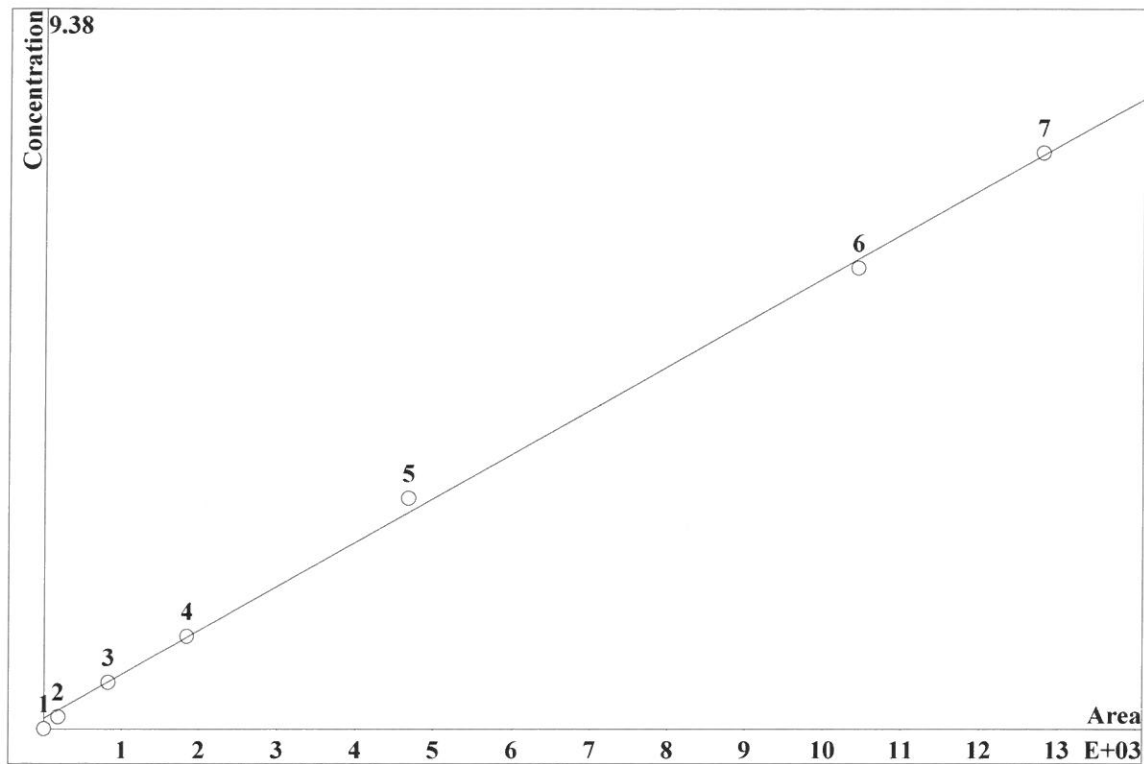


K3 = 0 K2 = 0 K1 = 0.0114575 K0 = 2.72962
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	10.14	184.9	0.15	20	11.64		
3	42.66	829.4	0.6	20	11.64		
4	94.06	1841	1.2	20	11.64		
5	237.6	4680	3	20	11.64		
6	535.3	1.044e+04	6	20	11.64		
7	650.7	1.28e+04	7.5	20	11.64		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-011419.mtw
 Equation: $Q = 0.060899 \cdot A + 5.50902$
 RSD: 3.653 %
 Correlation coefficient: 0.999455

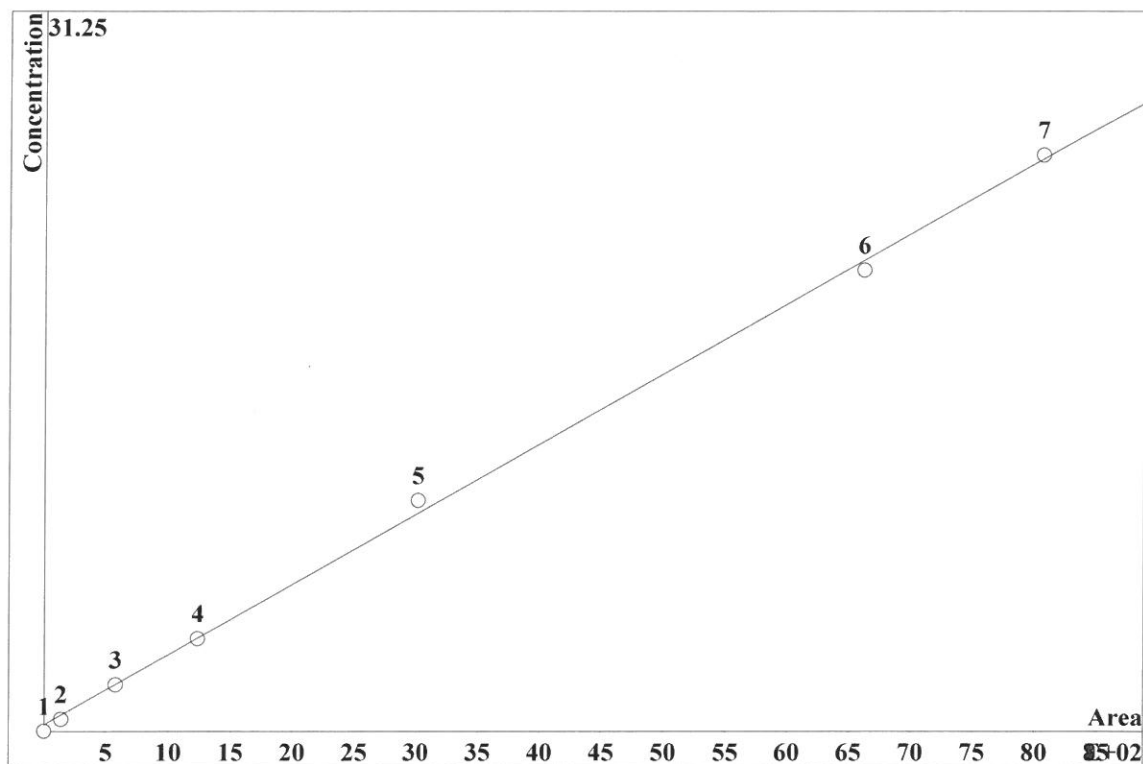

K3 = 0 K2 = 0 K1 = 0.060899 K0 = 5.50902

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.875	141.1	0.5	20	15.43		
3	19.57	575.5	2	20	15.43		
4	41.86	1237	4	20	15.43		
5	101.4	3015	10	20	15.43		
6	221.3	6621	20	20	15.43		
7	268.1	8065	25	20	15.43		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-011419.mtw
 Equation: $Q = 0.0109329 \cdot A + 1.36317$
 RSD: 3.838 %
 Correlation coefficient: 0.999399

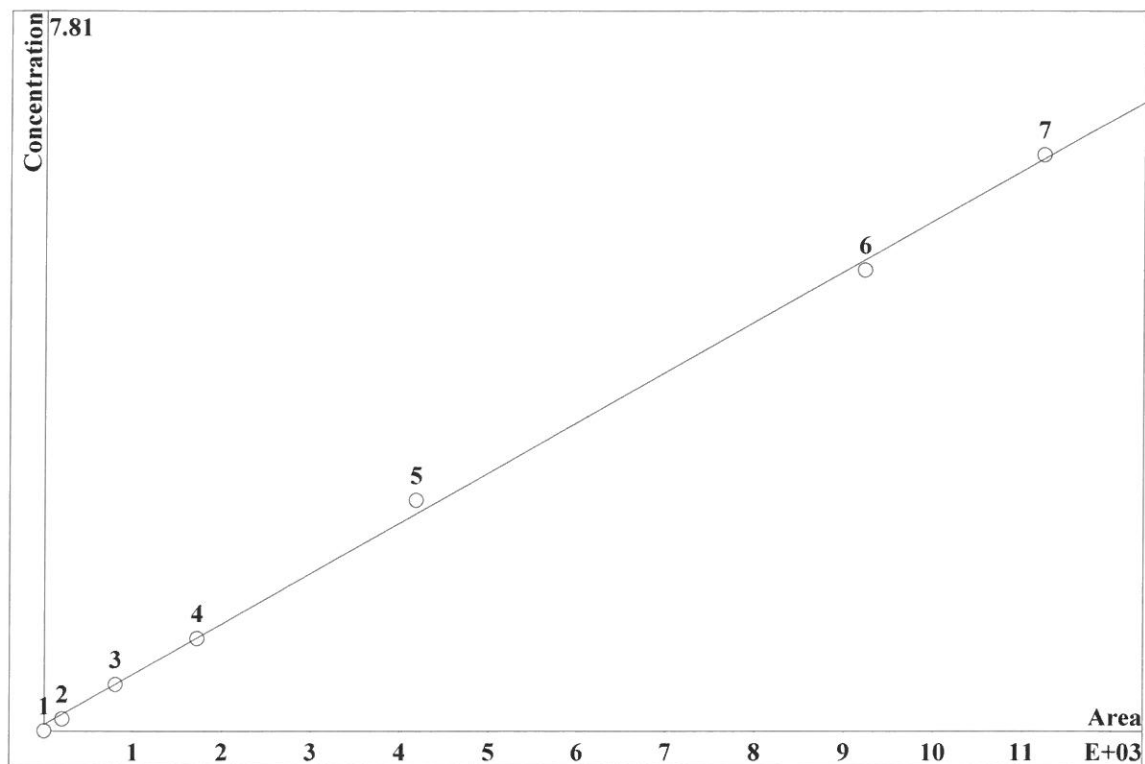

K3 = 0 K2 = 0 K1 = 0.0109329 K0 = 1.36317

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.906	205.8	0.125	20	18.5		
3	22.77	803.9	0.5	20	18.5		
4	47.75	1724	1	20	18.5		
5	112.7	4184	2.5	20	18.5		
6	237.9	9229	5	20	18.5		
7	285.2	1.123e+04	6.25	20	18.5		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-011419.mtw
 Equation: $Q = 0.0255618 \cdot A - 16.4708$
 RSD: 8.017 %
 Correlation coefficient: 0.997373

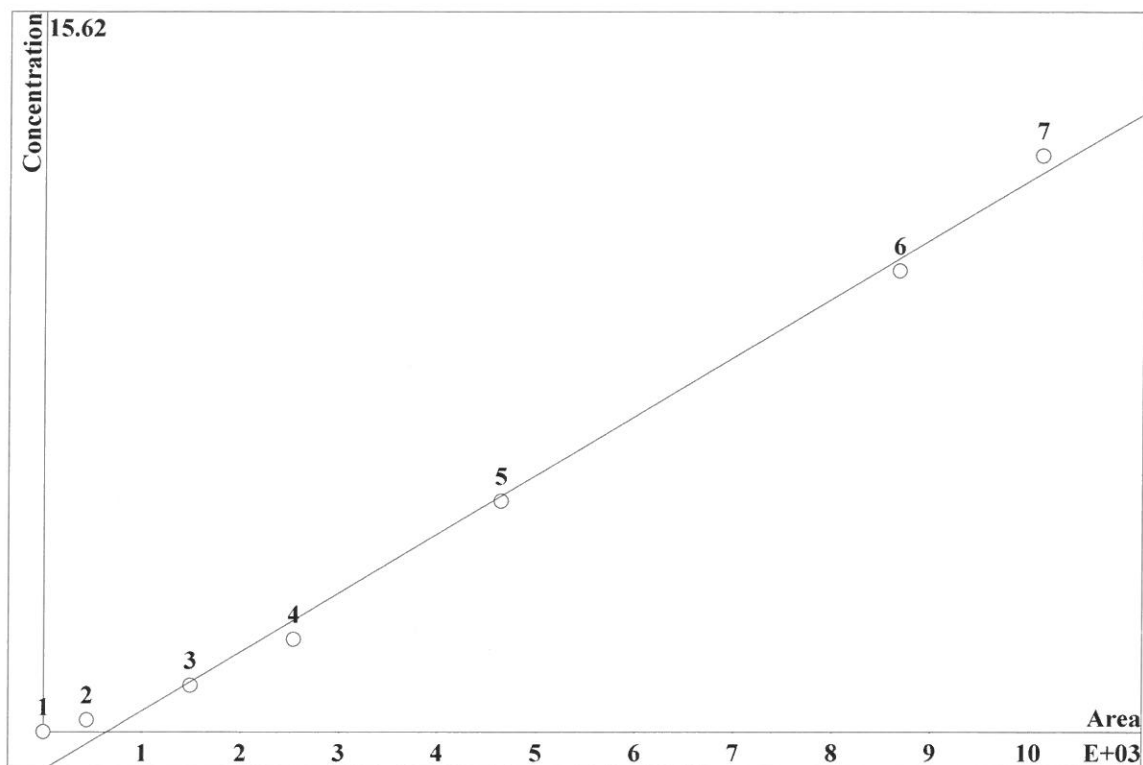


K3 = 0 K2 = 0 K1 = 0.0255618 K0 = -16.4708
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	9.127	441.8	0.25	20	23.19		
3	32.09	1491	1	20	23.19		
4	55.86	2539	2	20	23.19		
5	104.9	4646	5	20	23.19		
6	201.7	8681	10	20	23.19		
7	235.3	1.013e+04	12.5	20	23.19		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-011419.mtw
 Equation: $Q = 0.0371072 \cdot A + 12.502$
 RSD: 4.410 %
 Correlation coefficient: 0.999206

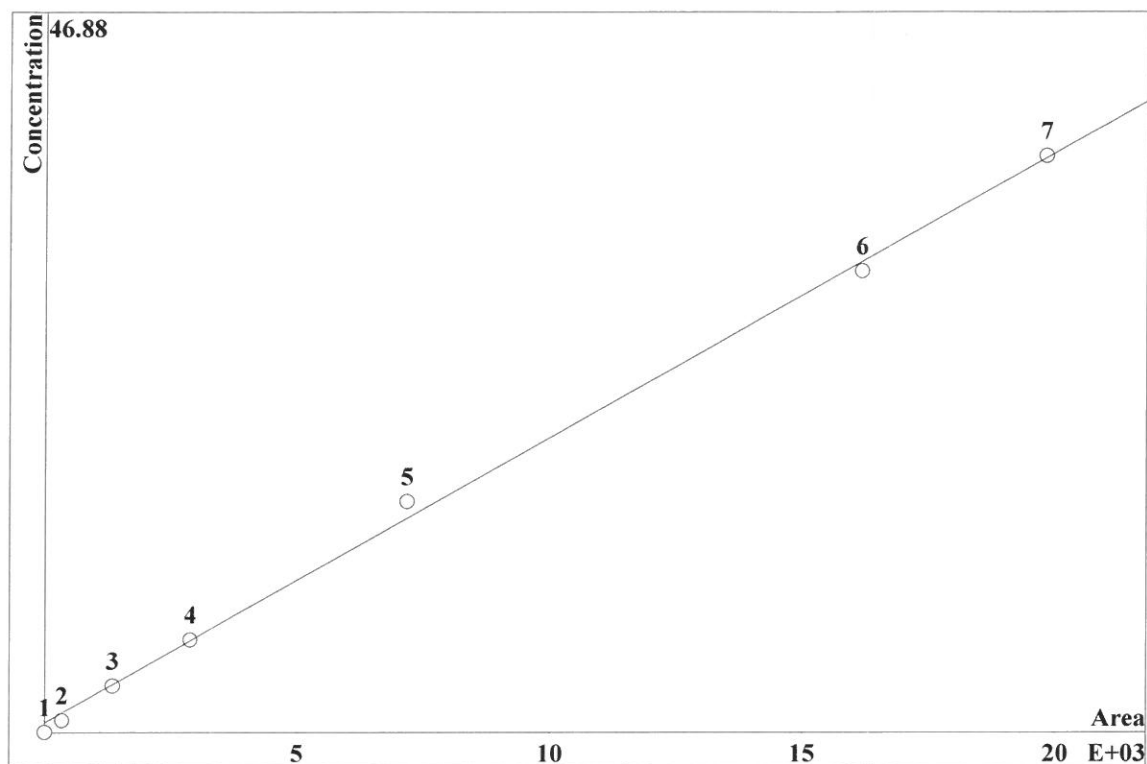

K3 = 0 K2 = 0 K1 = 0.0371072 K0 = 12.502

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.859	346.8	0.75	20	25.22		
3	33.72	1338	3	20	25.22		
4	71.87	2872	6	20	25.22		
5	177.7	7170	15	20	25.22		
6	399.8	1.617e+04	30	20	25.22		
7	487.1	1.98e+04	37.5	20	25.22		

a

Report date: 1/16/2019 1:21:52 PM
Printed by: wet


Ident: STD1
Analysis from: 1/14/2019 9:36:02 AM
File: _2019-01-14_

Last save: 1/14/2019 2:23:38 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19568

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

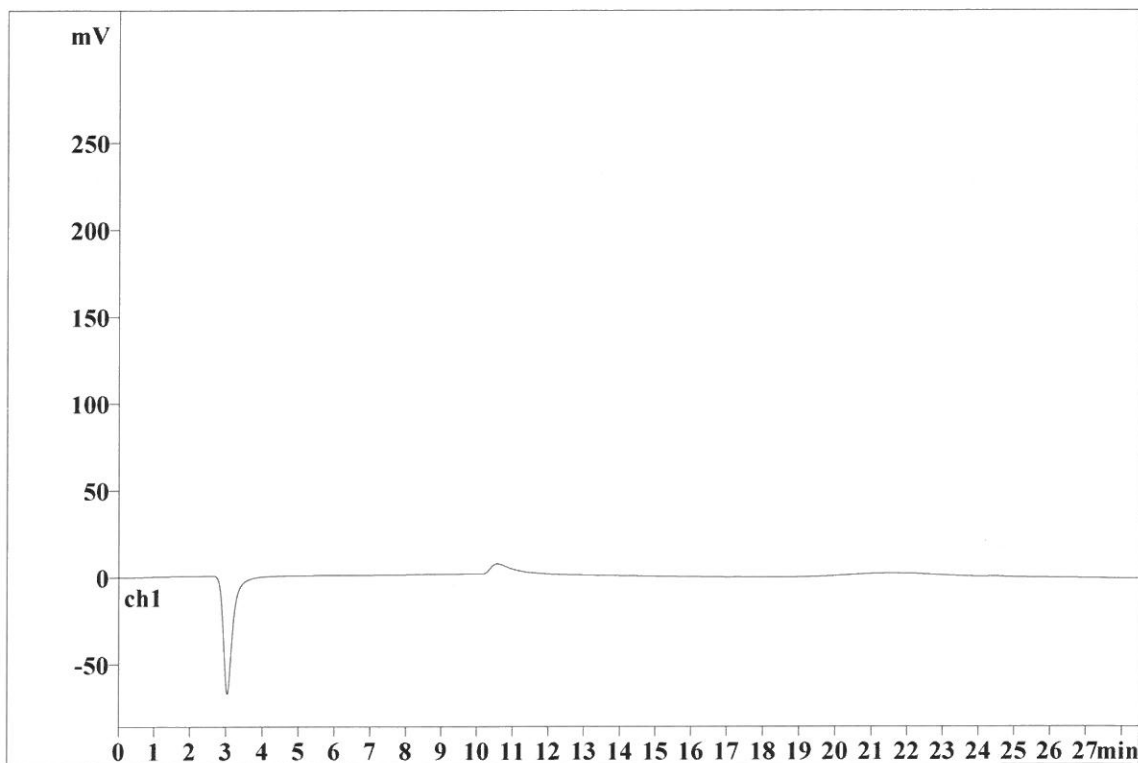

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:22:08 PM
Printed by: wet


Ident: STD2
Analysis from: 1/14/2019 10:07:27 AM
File: _2019-01-14_

Last save: 1/14/2019 2:23:38 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19569

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

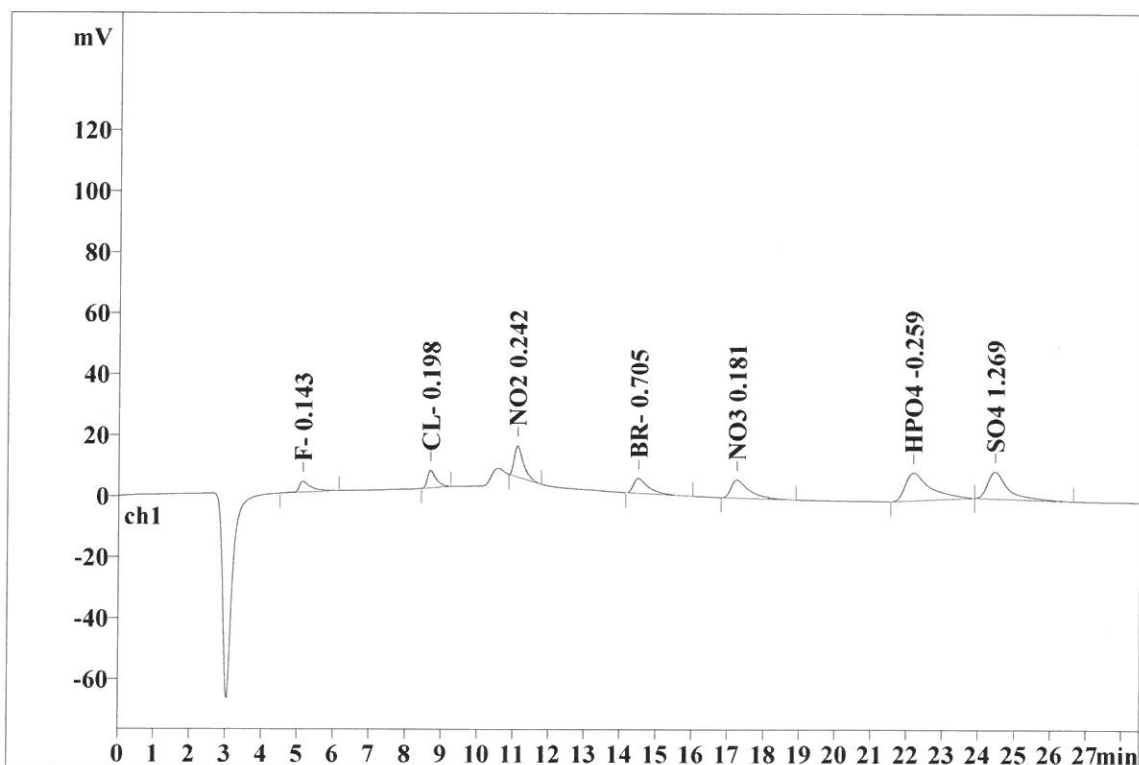

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.13	0.312	3.54	7.35	82.422	5.50
2	8.68	0.245	5.78	11.98	96.573	6.44
3	11.11	0.269	10.14	21.02	184.913	12.33
4	14.50	0.409	4.87	10.11	141.066	9.41
5	17.25	0.490	5.90	12.24	205.756	13.72
6	22.17	0.660	9.12	18.92	441.839	29.47
7	24.45	0.519	8.86	18.37	346.844	23.13
7	28.50	0.415	48.22	99.99	1499.412	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:22:18 PM
Printed by: wet


Ident: STD3
Analysis from: 1/14/2019 10:38:53 AM
File: _2019-01-14_

Last save: 1/14/2019 2:23:38 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19570

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

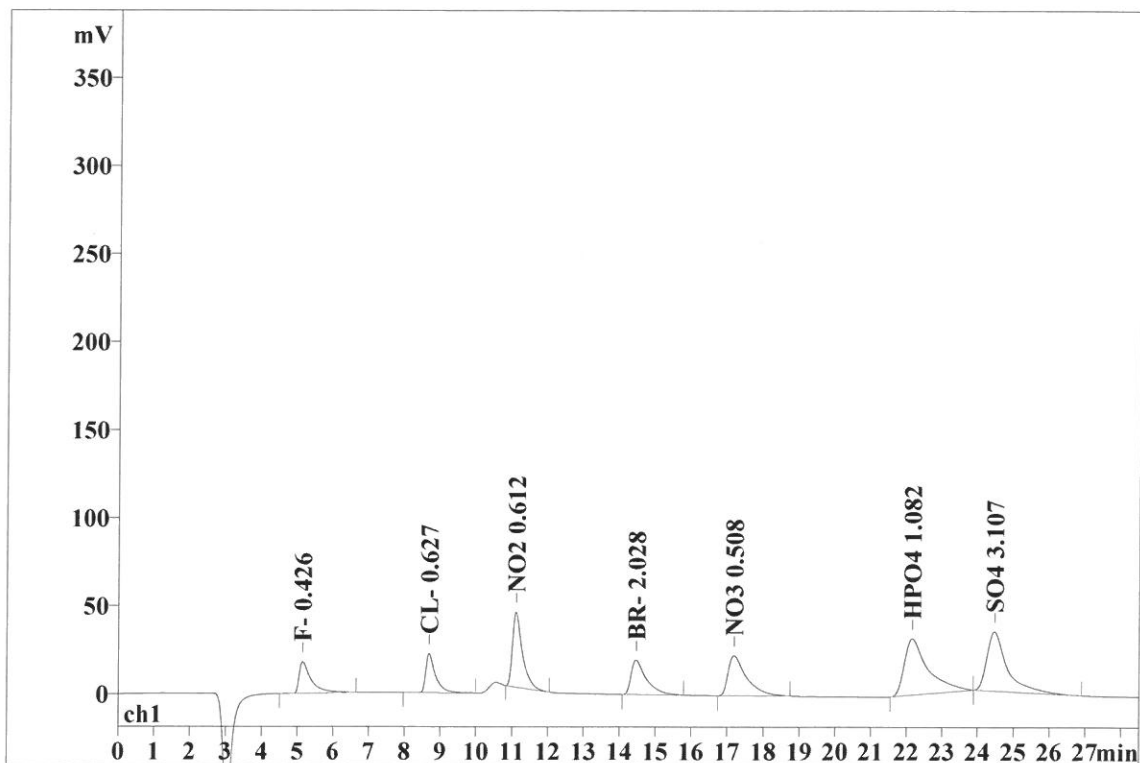

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.14	0.309	17.90	9.38	417.671	7.12
2	8.69	0.257	22.20	11.63	414.883	7.07
3	11.11	0.276	42.66	22.34	829.437	14.13
4	14.47	0.414	19.57	10.25	575.490	9.80
5	17.19	0.498	22.77	11.93	803.895	13.70
6	22.16	0.621	32.09	16.81	1490.874	25.40
7	24.47	0.522	33.72	17.66	1337.550	22.79
7	28.50	0.414	190.91	99.99	5869.799	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:22:29 PM
Printed by: wet


Ident: STD4
Analysis from: 1/14/2019 11:10:19 AM
File: _2019-01-14_

Last save: 1/14/2019 2:23:38 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19571

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

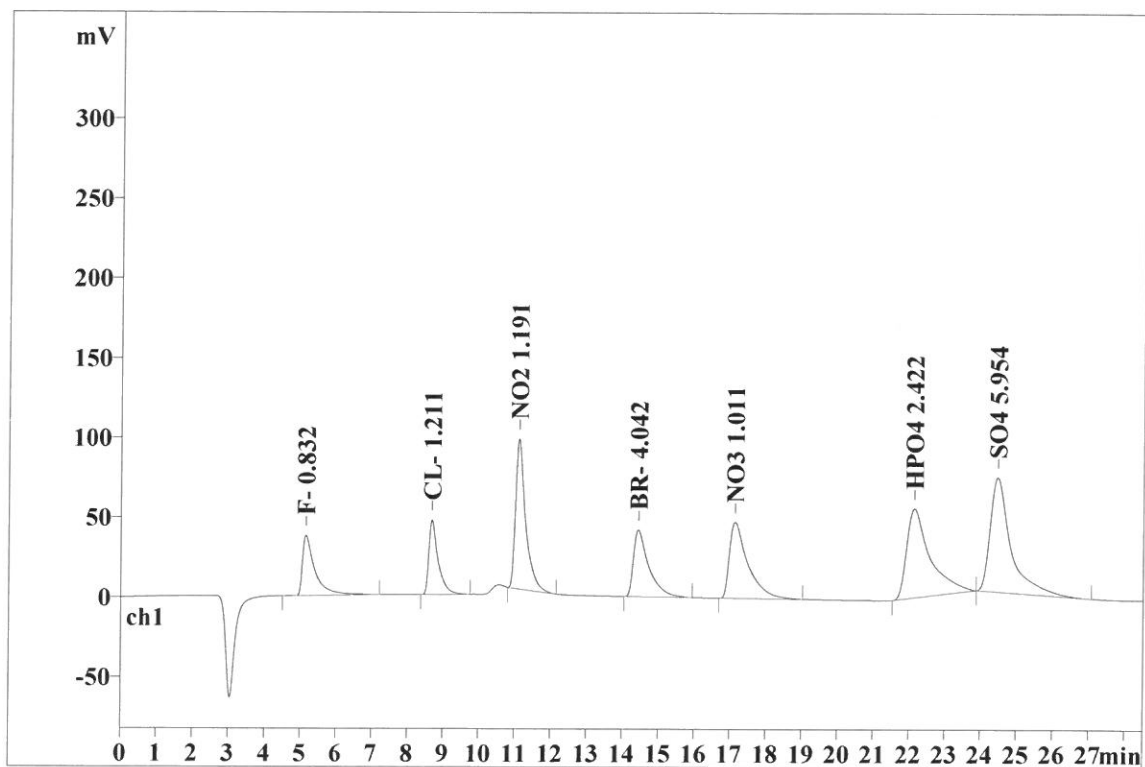

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.15	0.309	37.75	9.54	899.176	7.52
2	8.69	0.252	46.78	11.81	847.720	7.09
3	11.12	0.273	94.06	23.76	1841.013	15.39
4	14.44	0.411	41.86	10.57	1236.963	10.34
5	17.14	0.503	47.75	12.06	1723.932	14.41
6	22.14	0.605	55.86	14.11	2539.350	21.23
7	24.47	0.521	71.87	18.15	2872.249	24.01
7	28.50	0.411	395.93	100.00	11960.404	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:22:41 PM
Printed by: wet


Ident: STD5
Analysis from: 1/14/2019 11:41:45 AM
File: _2019-01-14_

Last save: 1/14/2019 2:23:38 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19572

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

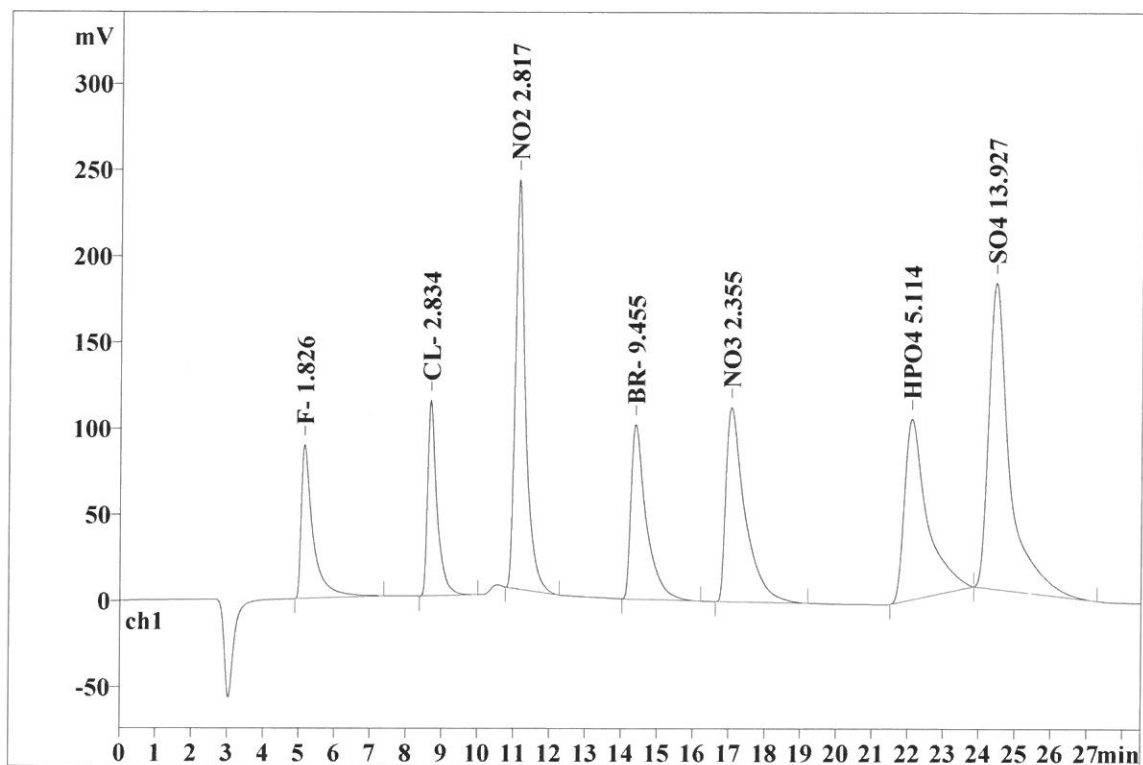

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.15	0.302	89.09	9.51	2077.214	7.47
2	8.68	0.252	113.37	12.10	2050.544	7.37
3	11.12	0.272	237.60	25.37	4679.552	16.82
4	14.39	0.412	101.37	10.82	3014.810	10.84
5	17.06	0.521	112.67	12.03	4184.127	15.04
6	22.10	0.589	104.87	11.20	4645.880	16.70
7	24.45	0.520	177.70	18.97	7169.631	25.77
7	28.50	0.410	936.67	100.00	27821.758	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:22:52 PM
Printed by: wet


Ident: STD6
Analysis from: 1/14/2019 12:13:10 PM
File: _2019-01-14_

Last save: 1/14/2019 2:23:38 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19573

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

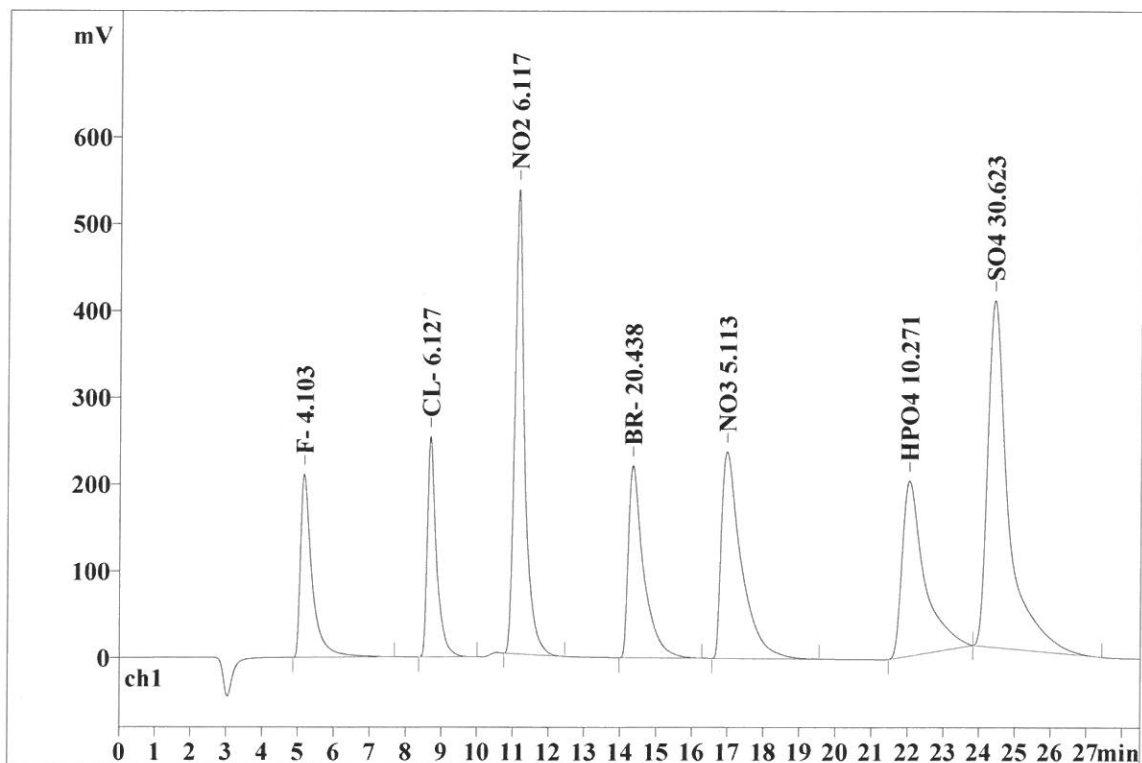

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.16	0.306	211.24	10.25	4777.447	7.91
2	8.68	0.245	253.90	12.32	4490.724	7.43
3	11.15	0.267	535.29	25.97	10439.065	17.28
4	14.34	0.415	221.29	10.74	6621.473	10.96
5	16.98	0.550	237.87	11.54	9228.550	15.28
6	22.04	0.573	201.73	9.79	8680.861	14.37
7	24.42	0.519	399.76	19.40	16168.465	26.77
7	28.50	0.411	2061.08	100.00	60406.586	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:23:02 PM
Printed by: wet


Ident: STD7
Analysis from: 1/14/2019 12:44:35 PM
File: _2019-01-14_

Last save: 1/14/2019 2:23:53 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19574

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

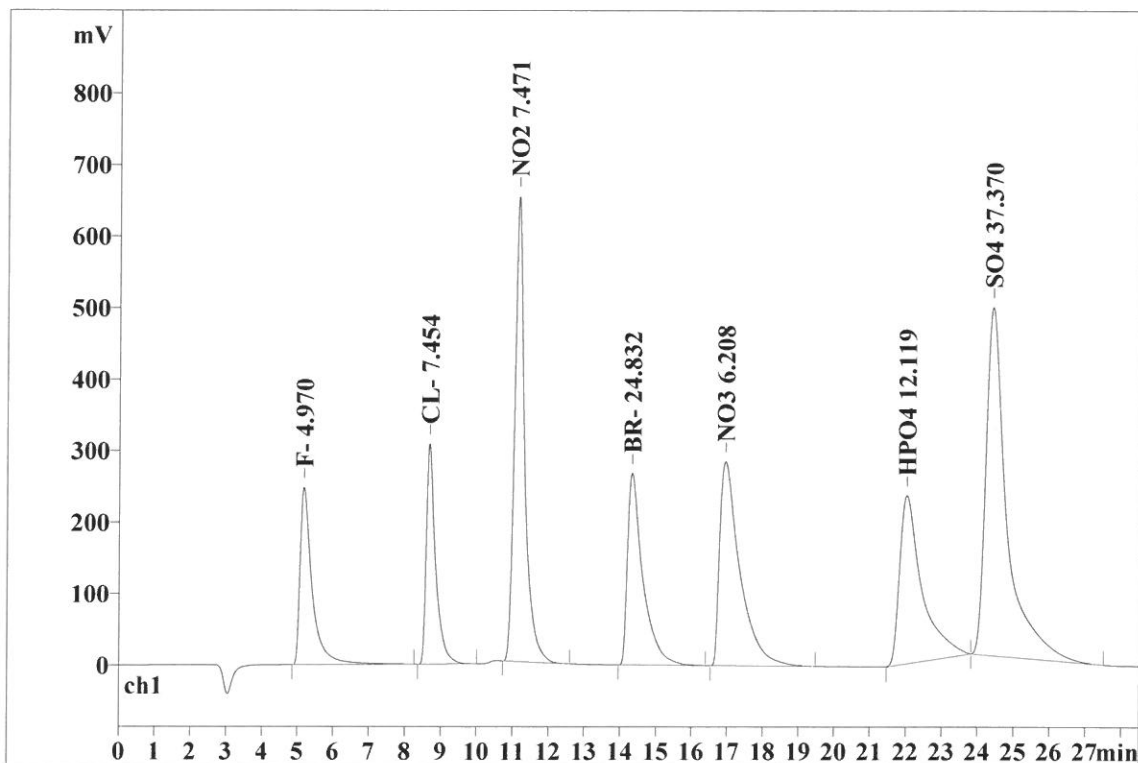

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.17	0.315	247.64	9.98	5805.210	7.92
2	8.68	0.246	308.18	12.41	5474.401	7.47
3	11.15	0.269	650.67	26.21	12802.674	17.46
4	14.32	0.416	268.09	10.80	8064.804	11.00
5	16.94	0.560	285.20	11.49	11231.677	15.32
6	22.02	0.575	235.30	9.48	10126.698	13.81
7	24.41	0.522	487.12	19.62	19804.577	27.01
7	28.50	0.415	2482.21	100.00	73310.041	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:27:53 PM
Printed by: wet


Ident: ICV
Analysis from: 1/14/2019 2:18:53 PM
File: _2019-01-14_

Last save: 1/15/2019 9:21:42 AM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19577

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

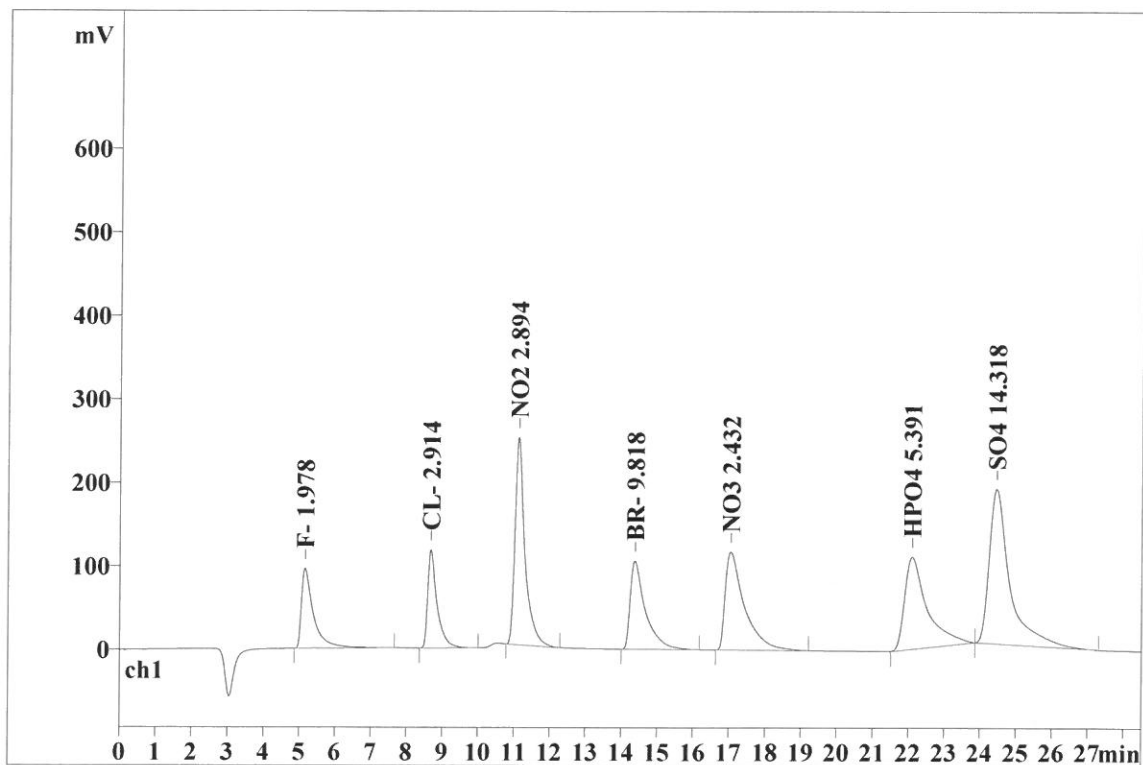

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.16	0.312	95.72	9.76	2258.367	7.84
2	8.68	0.247	117.41	11.98	2110.977	7.33
3	11.12	0.263	248.41	25.34	4814.299	16.72
4	14.38	0.400	105.57	10.77	3115.955	10.82
5	17.05	0.504	117.37	11.97	4322.411	15.01
6	22.09	0.577	110.36	11.26	4796.548	16.66
7	24.46	0.514	185.31	18.91	7376.427	25.62
7	28.50	0.402	980.17	100.00	28794.983	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/16/2019 1:28:02 PM
Printed by: wet


Ident: ICB
Analysis from: 1/14/2019 2:54:05 PM
File: _2019-01-14_

Last save: 1/15/2019 9:21:42 AM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19578

Last save: 1/14/2019 8:30:

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

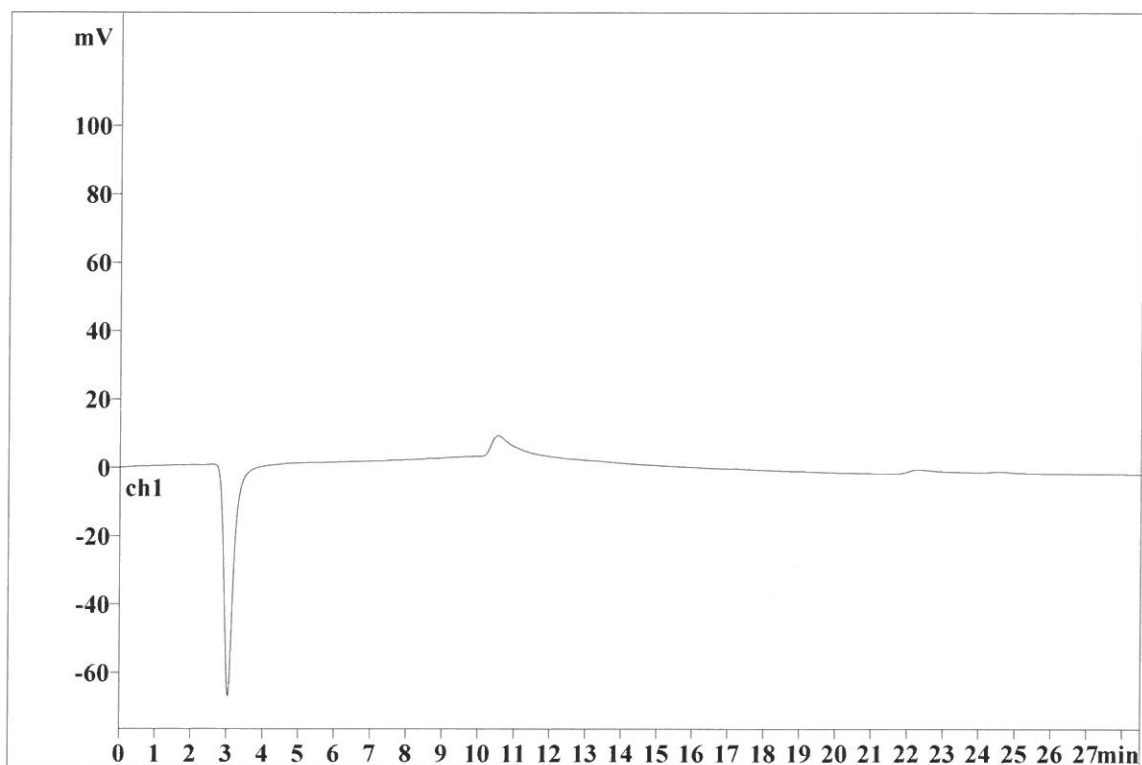

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:57:19 PM
Printed by: wet


Ident: CCV
Analysis from: 1/16/2019 7:52:16 AM
File: _2019-01-16_

Last save: 1/16/2019 8:20:46 AM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19589

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

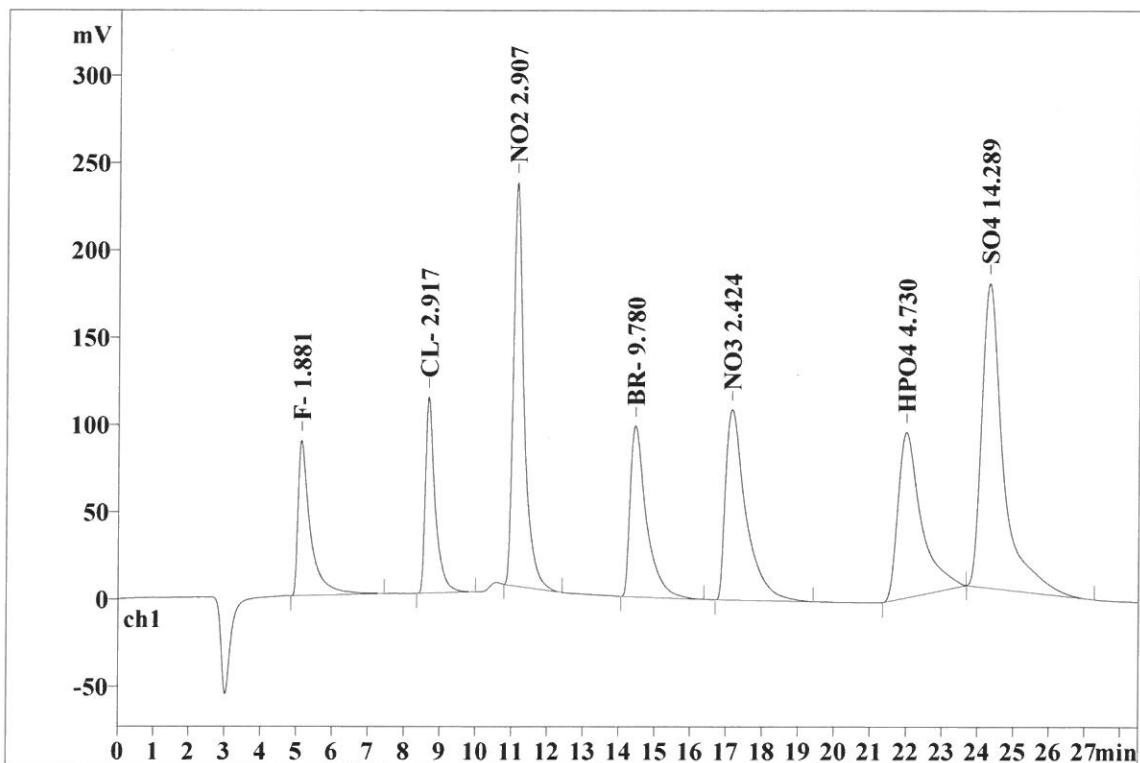

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.13	0.314	88.93	9.79	2142.812	7.62
2	8.68	0.262	112.31	12.36	2112.485	7.51
3	11.14	0.294	231.08	25.44	4835.986	17.19
4	14.45	0.445	97.93	10.78	3103.369	11.03
5	17.15	0.560	109.03	12.00	4308.028	15.32
6	21.99	0.626	94.75	10.43	4265.253	15.16
7	24.32	0.563	174.42	19.20	7360.654	26.17
7	28.50	0.438	908.44	100.00	28128.585	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:57:27 PM
Printed by: wet


Ident: CCB
Analysis from: 1/16/2019 8:34:21 AM
File: _2019-01-16_

Last save: 1/16/2019 9:02:51 AM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19590

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

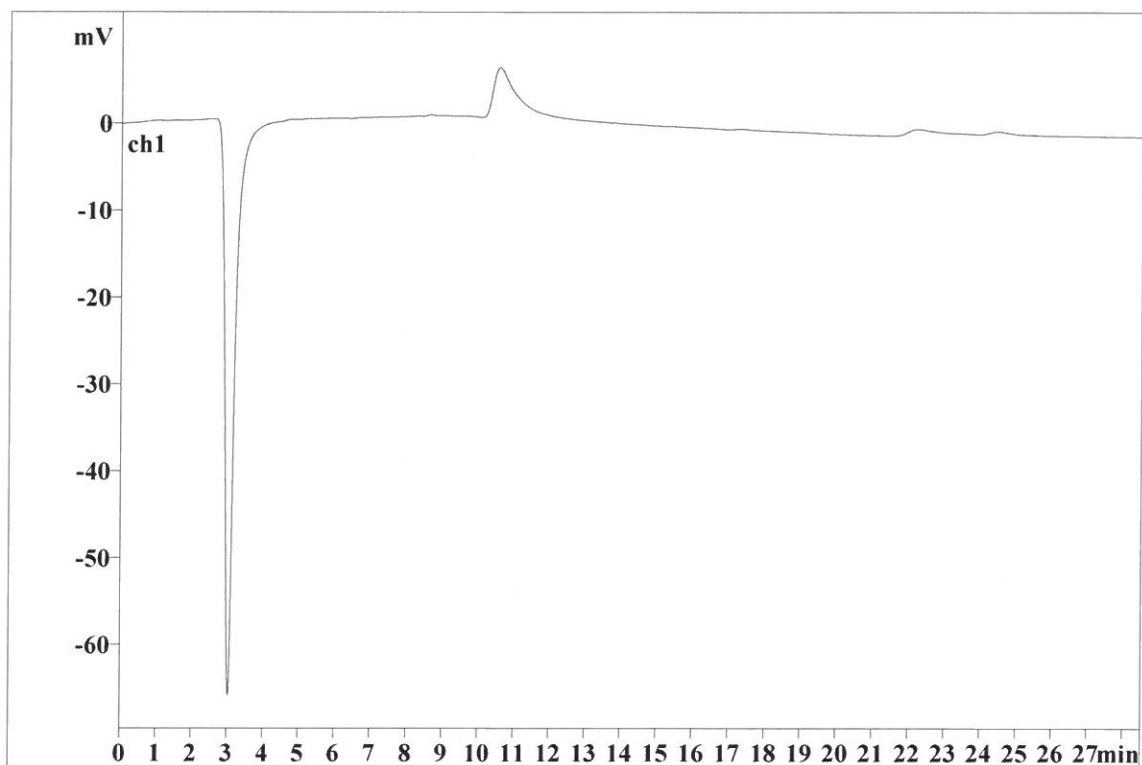

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:57:33 PM
Printed by: wet


Ident: LB100364BLW
Analysis from: 1/16/2019 9:05:46 AM
File: _2019-01-16_

Last save: 1/17/2019 2:56:17 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19591

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

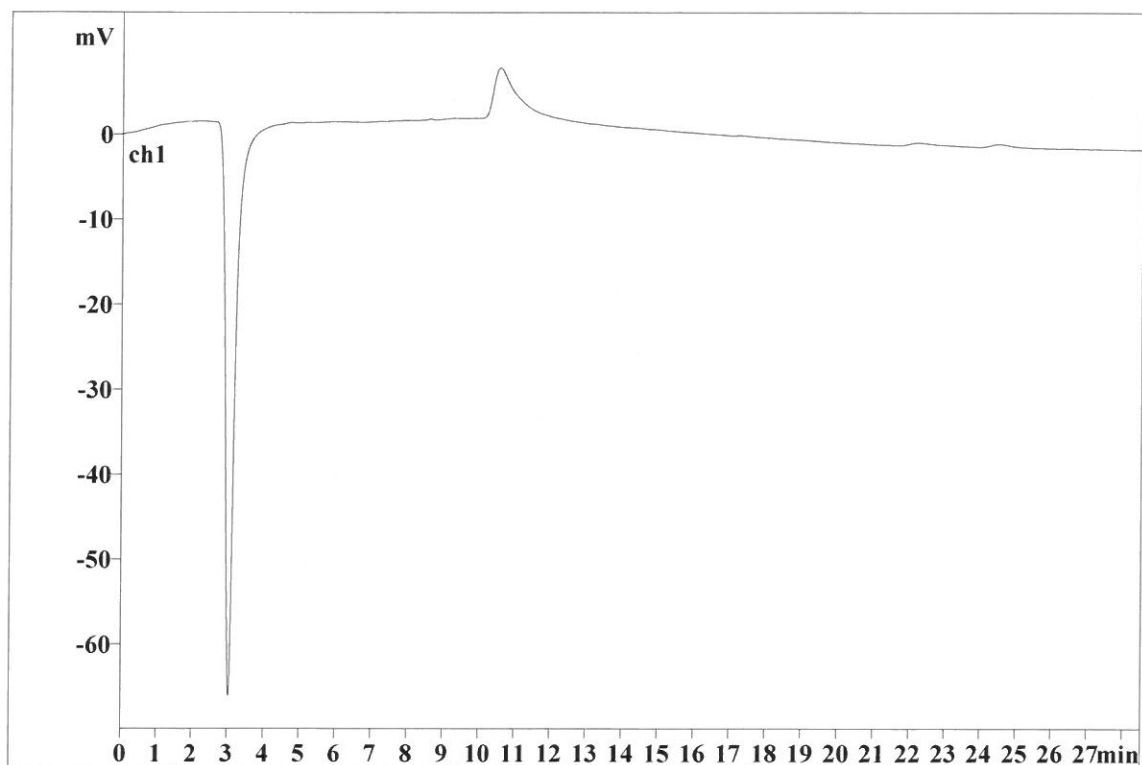

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:57:40 PM
Printed by: wet


Ident: LB100364BSW
Analysis from: 1/16/2019 9:37:12 AM
File: _2019-01-16_

Last save: 1/17/2019 2:56:17 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19592

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

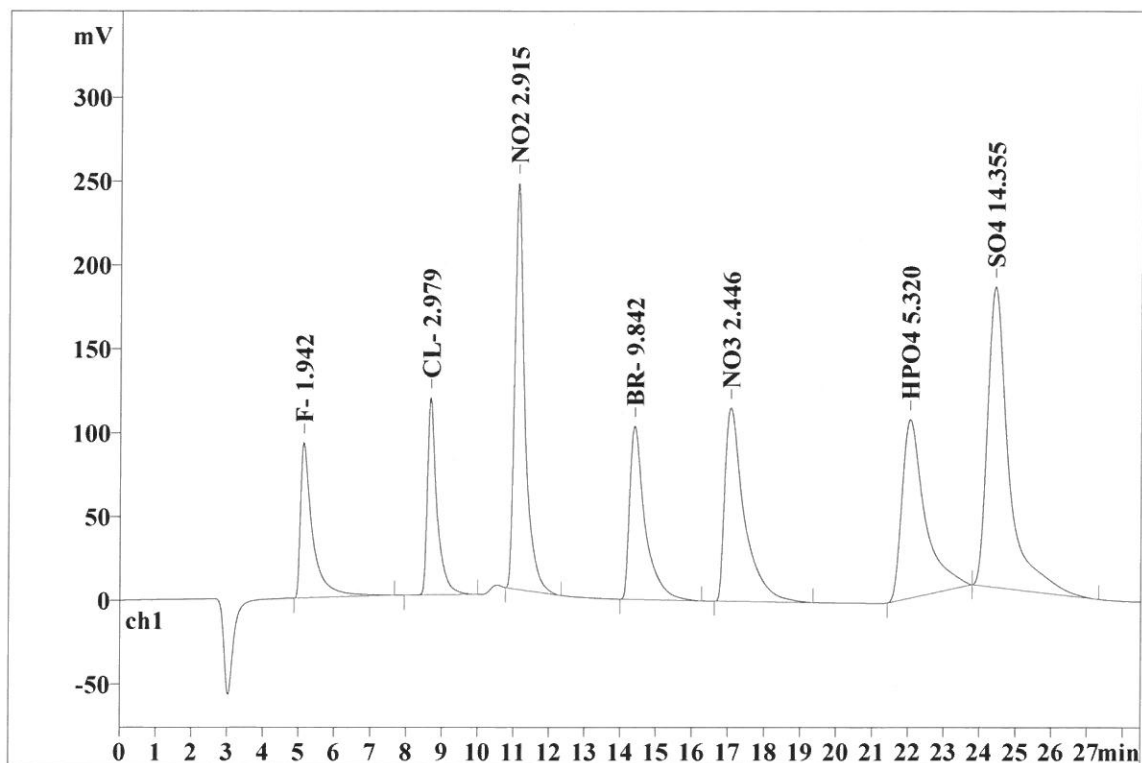

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.14	0.306	92.61	9.68	2214.946	7.68
2	8.67	0.249	117.59	12.29	2158.579	7.49
3	11.12	0.276	242.25	25.31	4851.017	16.83
4	14.39	0.413	103.35	10.80	3123.702	10.83
5	17.07	0.518	115.47	12.06	4347.906	15.08
6	22.04	0.611	106.57	11.13	4739.407	16.44
7	24.42	0.550	179.23	18.73	7396.124	25.65
7	28.50	0.418	957.07	100.00	28831.680	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:58:07 PM
Printed by: wet


Ident: K1166-01
Analysis from: 1/16/2019 4:29:43 PM
File: _2019-01-16_

Last save: 1/16/2019 4:58:13 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19595

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

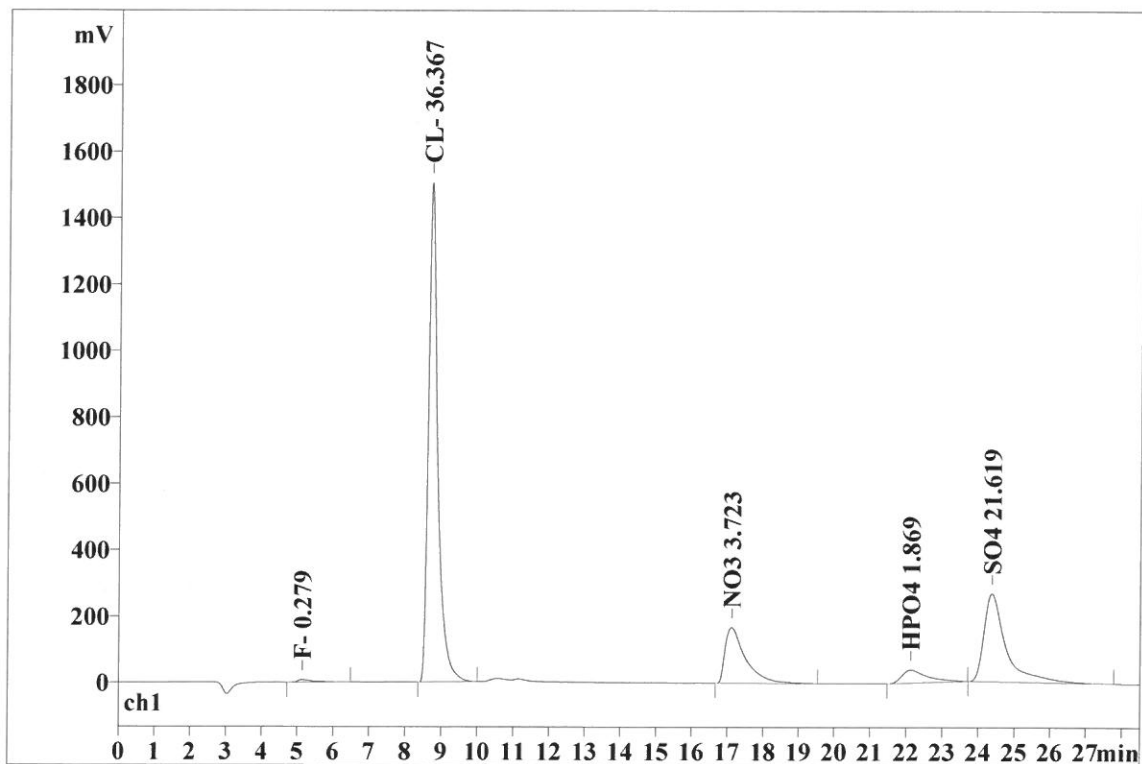

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.14	0.390	8.04	0.41	243.479	0.52
2	8.70	0.248	1504.41	75.79	26894.802	57.10
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.12	0.558	167.78	8.45	6684.785	14.19
6	22.13	0.714	39.30	1.98	1967.662	4.18
7	24.38	0.556	265.40	13.37	11313.170	24.02
7	28.50	0.352	1984.94	100.00	47103.897	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:58:58 PM
Printed by: wet


Ident: K1166-02
Analysis from: 1/16/2019 5:01:09 PM
File: _2019-01-16_

Last save: 1/17/2019 2:58:56 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19596

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

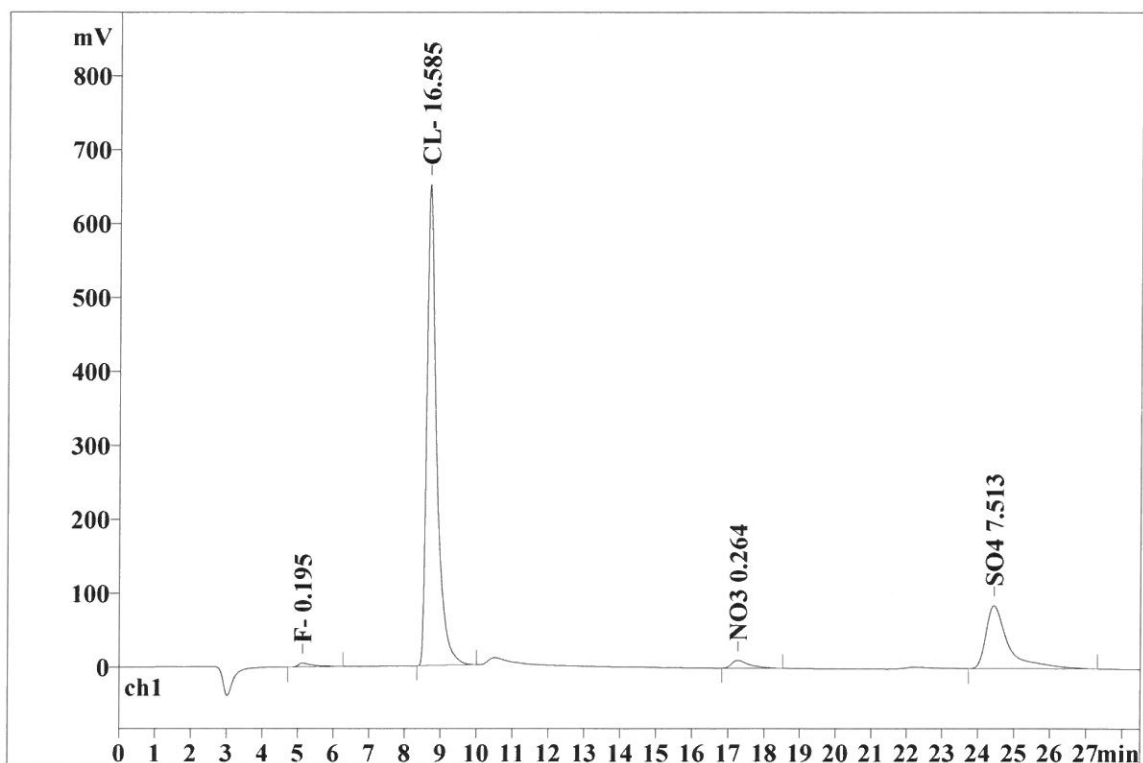

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.13	0.371	5.15	0.69	144.228	0.88
2	8.69	0.262	650.83	86.61	12239.027	74.42
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.27	0.493	10.34	1.38	355.508	2.16
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.45	0.561	85.14	11.33	3706.810	22.54
7	28.50	0.241	751.47	100.00	16445.573	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:59:06 PM
Printed by: wet


Ident: K1166-01DUP
Analysis from: 1/16/2019 5:32:35 PM
File: _2019-01-16_

Last save: 1/17/2019 2:58:38 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19597

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

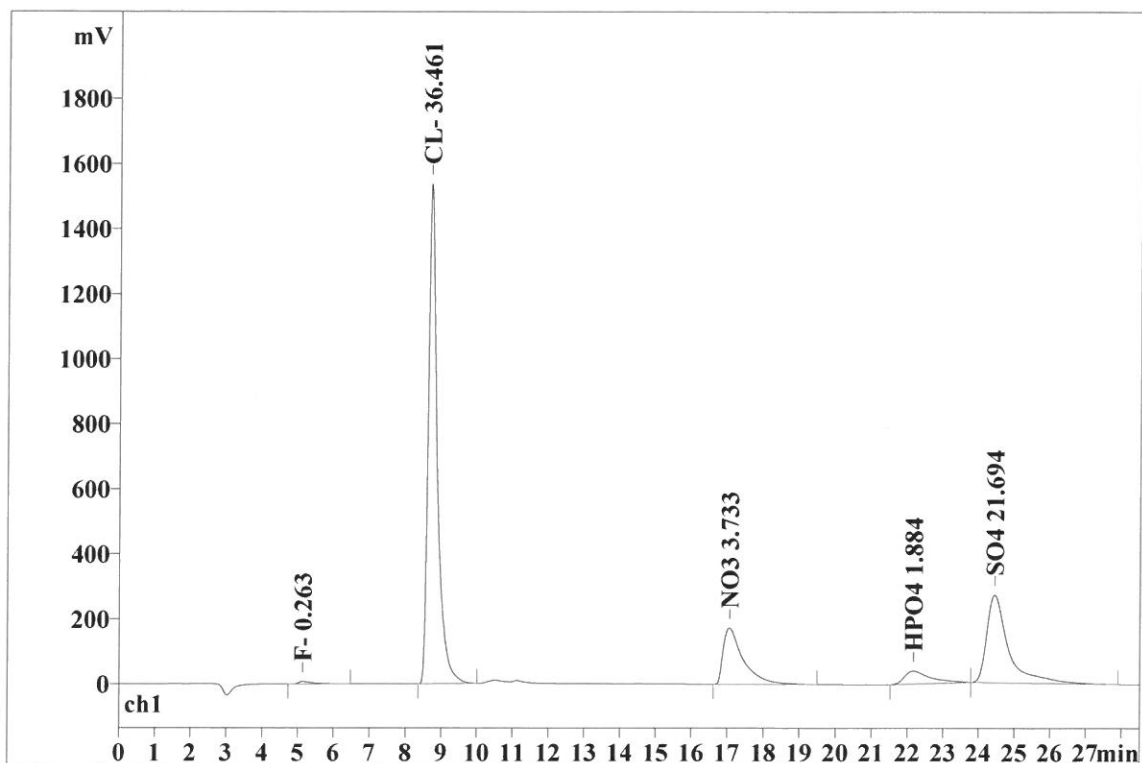

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.14	0.364	8.09	0.40	224.530	0.48
2	8.70	0.242	1536.86	75.81	26964.408	57.10
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.06	0.535	173.21	8.54	6703.133	14.19
6	22.16	0.704	39.76	1.96	1979.084	4.19
7	24.45	0.548	269.24	13.28	11353.641	24.04
7	28.50	0.342	2027.16	100.00	47224.797	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:59:13 PM
Printed by: wet


Ident: K1166-01MS
Analysis from: 1/16/2019 6:04:01 PM
File: _2019-01-16_

Last save: 1/16/2019 6:32:31 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19598

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

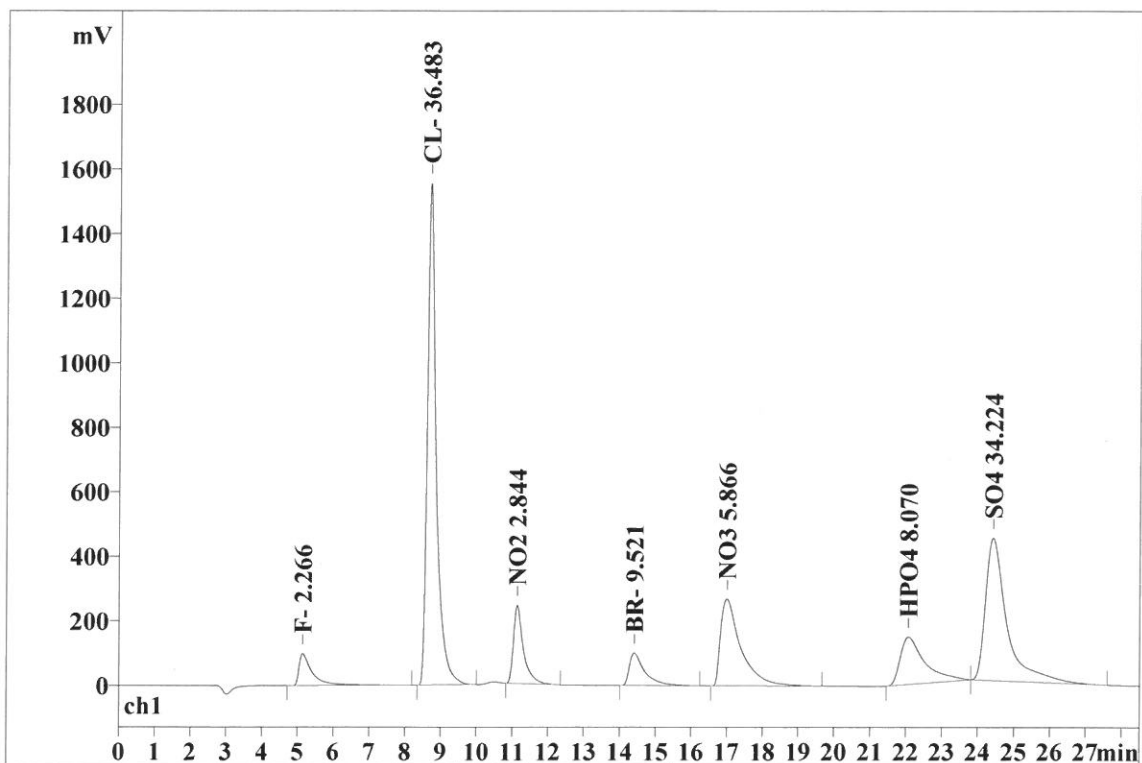

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.15	0.334	99.00	3.47	2599.670	3.56
2	8.69	0.238	1554.41	54.49	26980.598	36.97
3	11.14	0.268	242.51	8.50	4725.861	6.47
4	14.41	0.410	100.33	3.52	3017.661	4.13
5	17.00	0.546	268.83	9.42	10606.565	14.53
6	22.07	0.652	146.83	5.15	6948.270	9.52
7	24.43	0.543	440.80	15.45	18110.001	24.81
7	28.50	0.427	2852.71	100.00	72988.627	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:59:38 PM
Printed by: wet


Ident: K1166-01MSD
Analysis from: 1/16/2019 6:35:27 PM
File: _2019-01-16_

Last save: 1/16/2019 7:03:57 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19599

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

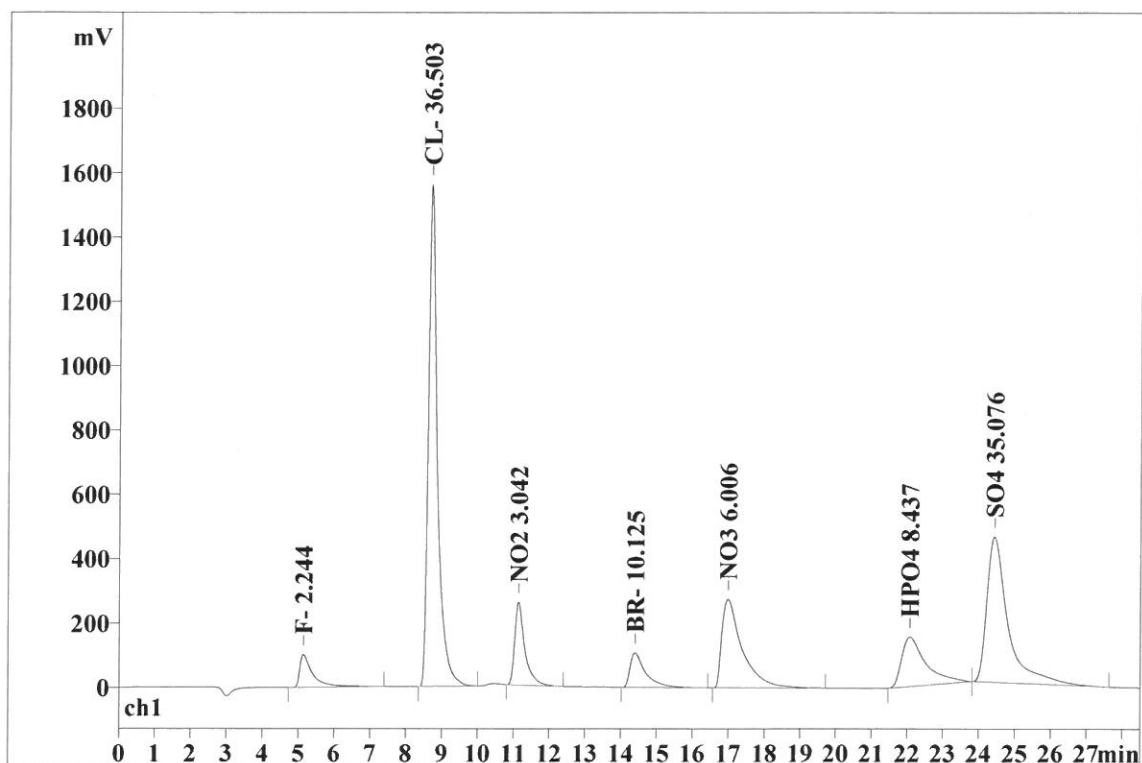

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.14	0.324	101.76	3.50	2573.126	3.45
2	8.69	0.236	1560.39	53.64	26994.967	36.22
3	11.14	0.269	257.96	8.87	5071.213	6.80
4	14.40	0.407	107.16	3.68	3217.271	4.32
5	16.98	0.544	275.10	9.46	10863.941	14.58
6	22.07	0.649	153.64	5.28	7243.465	9.72
7	24.44	0.542	452.92	15.57	18569.747	24.91
7	28.50	0.424	2908.93	99.99	74533.728	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:59:46 PM
Printed by: wet


Ident: CCV
Analysis from: 1/16/2019 7:07:00 PM
File: _2019-01-16_

Last save: 1/16/2019 7:35:30 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19600

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

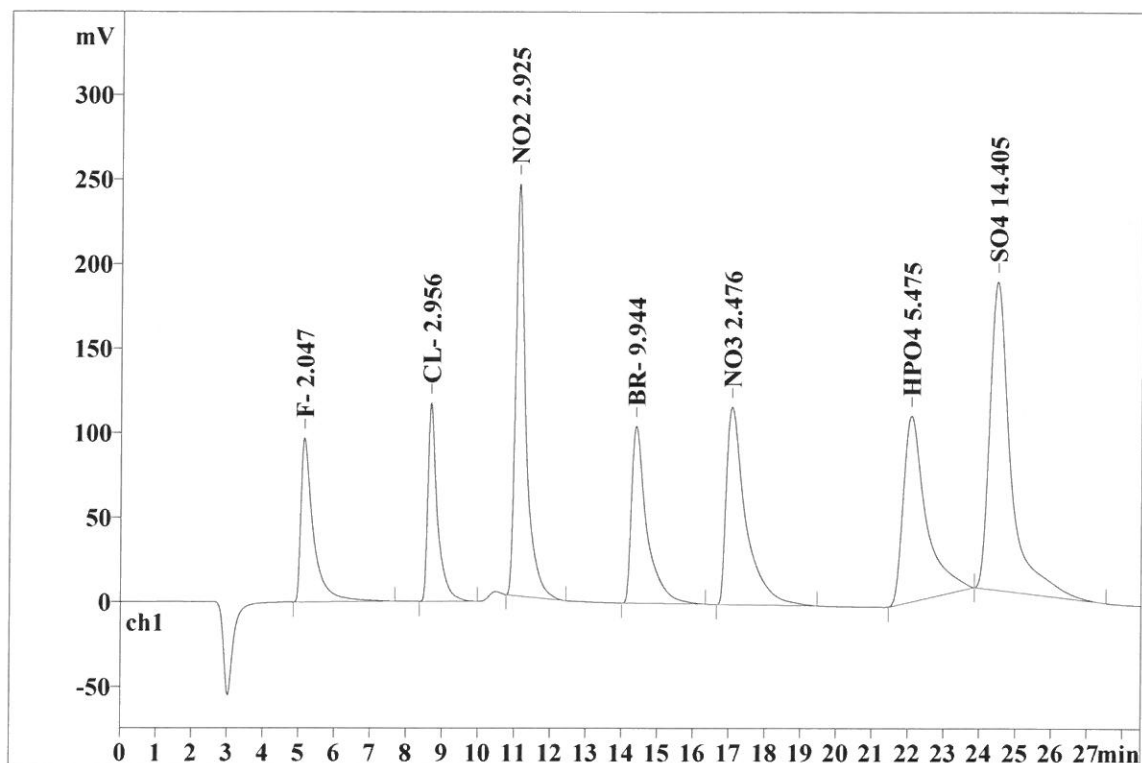

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.15	0.318	97.06	9.99	2339.765	8.01
2	8.68	0.245	117.35	12.07	2141.485	7.33
3	11.12	0.270	243.61	25.07	4867.762	16.67
4	14.40	0.405	104.58	10.76	3157.400	10.81
5	17.08	0.508	116.84	12.02	4403.872	15.08
6	22.08	0.603	110.03	11.32	4863.942	16.66
7	24.48	0.541	182.38	18.77	7423.526	25.42
7	28.50	0.413	971.86	100.00	29197.752	100.00

This report has been created by IC Net
METROHM LTD

Report date: 1/17/2019 2:59:56 PM
Printed by: wet


Ident: CCB
Analysis from: 1/16/2019 7:38:26 PM
File: _2019-01-16_

Last save: 1/16/2019 8:06:56 PM

Method: AnionsIC2-011419.mtw
Run operator: wet
Analysis number: 19601

Last save: 1/14/2019 3:31:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

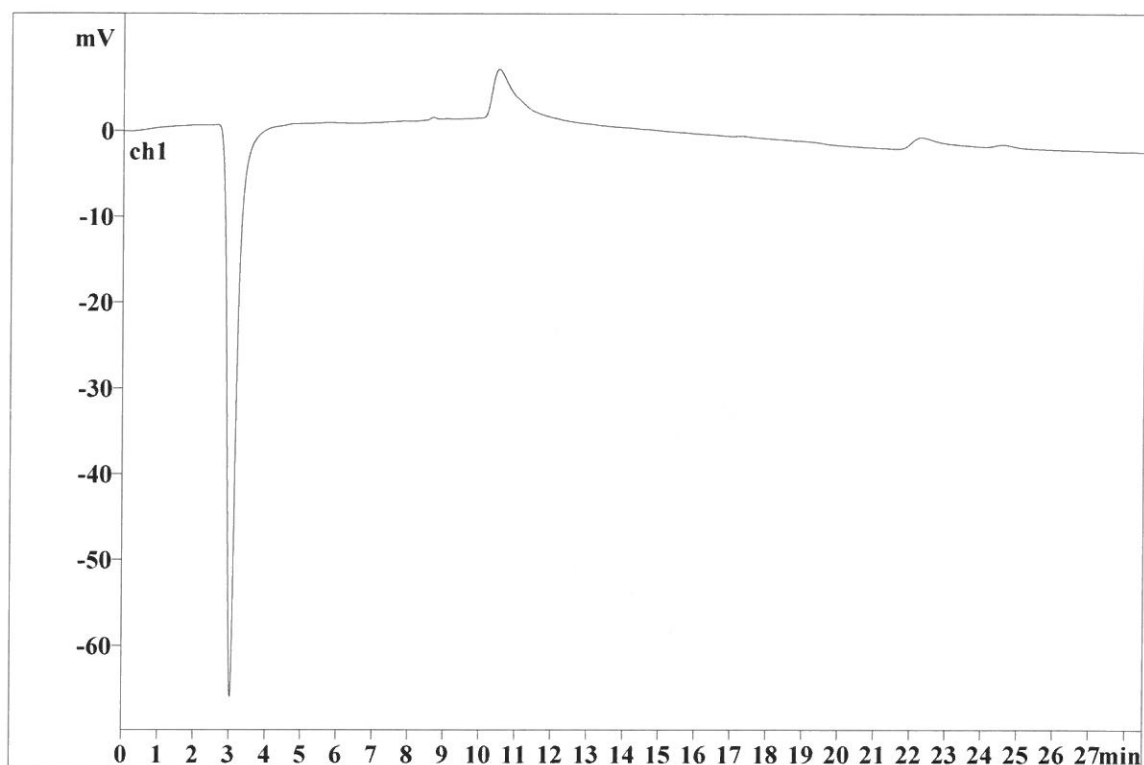

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD