

2B100389

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

1/18/2019 12:16

Test: *Detective*
~~Total~~ CN

Sample Id	<i>My R</i> Result	Dil. 1 +	Response	Errors
ICV1	98.009	0.0	0.090	
ICB1	0.249	0.0	0.004	
CCV1	244.027	0.0	0.217	
CCB1	-0.275	0.0	0.004	
PB116463BL	-0.373	0.0	0.004	
K1011-06	-0.207	0.0	0.004	
K1011-08	-0.628	0.0	0.004	
K1015-10	-0.319	0.0	0.004	
K1015-12	-0.364	0.0	0.004	
K1159-01	-0.357	0.0	0.004	
K1173-02	-0.482	0.0	0.004	
K1173-04	-0.420	0.0	0.004	
K1173-06	-0.446	0.0	0.004	
K1173-08	-0.375	0.0	0.004	
CCV2	244.607	0.0	0.217	
CCB2	-1.029	0.0	0.003	
K1180-02	-0.447	0.0	0.004	
K1189-02	-0.451	0.0	0.004	
K1189-04	-0.215	0.0	0.004	
K1189-04DUP	0.019	0.0	0.004	
CCV3	237.063	0.0	0.211	
CCB3	-0.059	0.0	0.004	

N 22
Mean 37.160
SD 85.8598
CV% 231.05

As

Aquakem v. 7.2AQ1

Results from time period:

Fri Jan 18 12:06:02 2019

Fri Jan 18 12:13:47 2019

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.741	µg/l	1/18/2019 9:45:26	
5.OPPBCN	A	Reactive CN	P	3.8904	µg/l	1/18/2019 9:45:27	
10PPBCN	A	Reactive CN	P	9.2978	µg/l	1/18/2019 9:45:28	
50PPBCN	A	Reactive CN	P	49.6592	µg/l	1/18/2019 9:45:29	
100PPBCN	A	Reactive CN	P	101.4128	µg/l	1/18/2019 9:45:30	
250PPBCN	A	Reactive CN	P	253.4084	µg/l	1/18/2019 9:45:31	
500PPBCN	A	Reactive CN	P	498.0724	µg/l	1/18/2019 9:45:32	
ICV1	S	Reactive CN	P	98.0087	µg/l	1/18/2019 12:06:02	
ICB1	S	Reactive CN	P	0.2495	µg/l	1/18/2019 12:06:03	
CCV1	S	Reactive CN	P	244.0274	µg/l	1/18/2019 12:06:04	
CCB1	S	Reactive CN	P	-0.2751	µg/l	1/18/2019 12:06:05	
PB116463BL	S	Reactive CN	P	-0.3735	µg/l	1/18/2019 12:06:06	
K1011-06	S	Reactive CN	P	-0.2065	µg/l	1/18/2019 12:06:07	
K1011-08	S	Reactive CN	P	-0.6283	µg/l	1/18/2019 12:06:08	
K1015-10	S	Reactive CN	P	-0.3186	µg/l	1/18/2019 12:06:09	
K1015-12	S	Reactive CN	P	-0.3643	µg/l	1/18/2019 12:06:10	
K1159-01	S	Reactive CN	P	-0.3572	µg/l	1/18/2019 12:06:11	
K1173-02	S	Reactive CN	P	-0.4817	µg/l	1/18/2019 12:06:12	
K1173-04	S	Reactive CN	P	-0.4196	µg/l	1/18/2019 12:13:37	
K1173-06	S	Reactive CN	P	-0.4458	µg/l	1/18/2019 12:13:38	
K1173-08	S	Reactive CN	P	-0.3748	µg/l	1/18/2019 12:13:39	
CCV2	S	Reactive CN	P	244.6072	µg/l	1/18/2019 12:13:40	
CCB2	S	Reactive CN	P	-1.0289	µg/l	1/18/2019 12:13:41	
K1180-02	S	Reactive CN	P	-0.4473	µg/l	1/18/2019 12:13:42	
K1189-02	S	Reactive CN	P	-0.4511	µg/l	1/18/2019 12:13:43	
K1189-04	S	Reactive CN	P	-0.2154	µg/l	1/18/2019 12:13:44	
K1189-04DUP	S	Reactive CN	P	0.0191	µg/l	1/18/2019 12:13:45	
CCV3	S	Reactive CN	P	237.0628	µg/l	1/18/2019 12:13:46	
CCB3	S	Reactive CN	P	-0.0586	µg/l	1/18/2019 12:13:47	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

1/18/2019 12:07


Test Total CN

Accepted 1/18/2019 9:47

Factor 1147
Bias 0.004

Coeff. of det. 0.999904

Errors

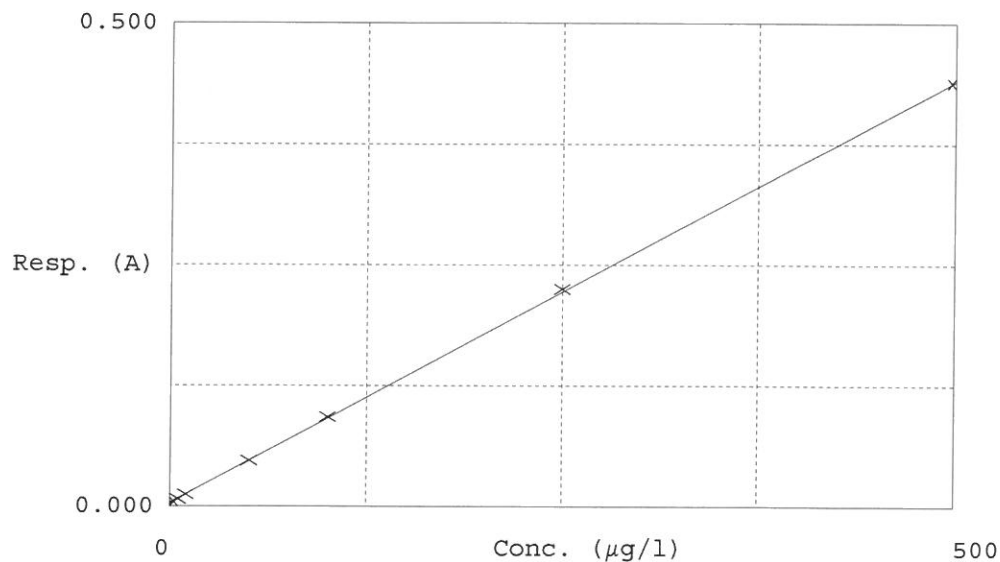

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.7410	0.0000	
2	5.0PPBCN	0.008	3.8904	5.0000	
3	10PPBCN	0.012	9.2978	10.0000	
4	50PPBCN	0.048	49.6592	50.0000	
5	100PPBCN	0.093	101.4128	100.0000	
6	250PPBCN	0.225	253.4084	250.0000	
7	500PPBCN	0.438	498.0724	500.0000	