

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : As

1/21/2019 14:32

Test: *Reactive* Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.757	0.0	0.089	
ICB1	0.530	0.0	0.004	
CCV1	239.738	0.0	0.219	
CCB1	0.207	0.0	0.004	
PB116529BL	0.369	0.0	0.004	
K1009-02	0.108	0.0	0.004	
K1009-02DUP	0.222	0.0	0.004	
K1009-04	0.101	0.0	0.004	
K1009-06	0.290	0.0	0.004	
K1009-08	0.145	0.0	0.004	
K1013-02	0.265	0.0	0.004	
K1013-04	-0.073	0.0	0.004	
K1013-06	0.124	0.0	0.004	
K1013-08	0.372	0.0	0.004	
CCV2	244.099	0.0	0.223	
CCB2	0.360	0.0	0.004	
PB116530BL	0.205	0.0	0.004	
K1200-02	0.368	0.0	0.004	
K1200-02DUP	0.513	0.0	0.004	
CCV3	249.377	0.0	0.228	
CCB3	0.777	0.0	0.004	

N	21
Mean	39.660
SD	88.0902
CV%	222.12

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

1/21/2019 12:57


Test Total CN

Accepted 1/21/2019 12:57

Factor 1112
Bias 0.004

Coeff. of det. 0.999968

Errors

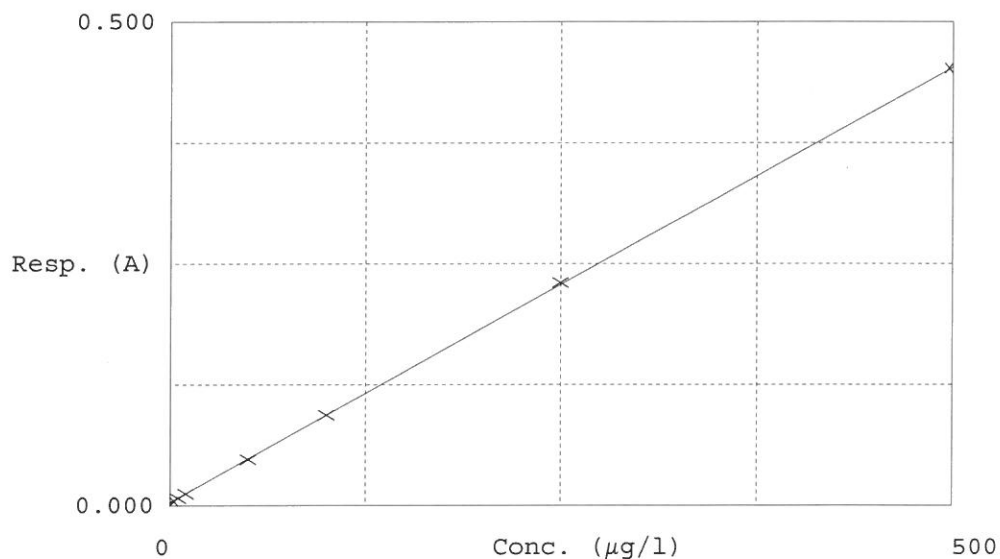

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.2335	0.0000	
2	5.0PPBCN	0.008	4.5103	5.0000	
3	10PPBCN	0.012	9.7653	10.0000	
4	50PPBCN	0.048	49.1763	50.0000	
5	100PPBCN	0.094	100.1925	100.0000	
6	250PPBCN	0.230	252.1371	250.0000	
7	500PPBCN	0.452	498.9849	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Mon Jan 21 14:19:37 2019

Mon Jan 21 14:26:53 2019

As

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.2335	µg/l	1/21/2019 12:57:14	
5.OPPBCN	A	Reactive CN	P	4.5103	µg/l	1/21/2019 12:57:15	
10PPBCN	A	Reactive CN	P	9.7653	µg/l	1/21/2019 12:57:16	
50PPBCN	A	Reactive CN	P	49.1763	µg/l	1/21/2019 12:57:17	
100PPBCN	A	Reactive CN	P	100.1925	µg/l	1/21/2019 12:57:18	
250PPBCN	A	Reactive CN	P	252.1371	µg/l	1/21/2019 12:57:19	
500PPBCN	A	Reactive CN	P	498.9849	µg/l	1/21/2019 12:57:20	
ICV1	S	Reactive CN	P	94.7566	µg/l	1/21/2019 14:19:37	
ICB1	S	Reactive CN	P	0.5303	µg/l	1/21/2019 14:19:38	
CCV1	S	Reactive CN	P	239.7384	µg/l	1/21/2019 14:19:39	
CCB1	S	Reactive CN	P	0.2073	µg/l	1/21/2019 14:19:40	
PB116529BL	S	Reactive CN	P	0.3688	µg/l	1/21/2019 14:19:41	
K1009-02	S	Reactive CN	P	0.108	µg/l	1/21/2019 14:19:42	
K1009-02DUP	S	Reactive CN	P	0.2218	µg/l	1/21/2019 14:19:43	
K1009-04	S	Reactive CN	P	0.1006	µg/l	1/21/2019 14:19:44	
K1009-06	S	Reactive CN	P	0.2899	µg/l	1/21/2019 14:19:45	
K1009-08	S	Reactive CN	P	0.1451	µg/l	1/21/2019 14:19:46	
K1013-02	S	Reactive CN	P	0.2646	µg/l	1/21/2019 14:19:47	
K1013-04	S	Reactive CN	P	-0.0725	µg/l	1/21/2019 14:26:44	
K1013-06	S	Reactive CN	P	0.1245	µg/l	1/21/2019 14:26:45	
K1013-08	S	Reactive CN	P	0.3721	µg/l	1/21/2019 14:26:46	
CCV2	S	Reactive CN	P	244.0992	µg/l	1/21/2019 14:26:47	
CCB2	S	Reactive CN	P	0.3596	µg/l	1/21/2019 14:26:48	
PB116530BL	S	Reactive CN	P	0.2052	µg/l	1/21/2019 14:26:49	
K1200-02	S	Reactive CN	P	0.3677	µg/l	1/21/2019 14:26:50	
K1200-02DUP	S	Reactive CN	P	0.5129	µg/l	1/21/2019 14:26:51	
CCV3	S	Reactive CN	P	249.3768	µg/l	1/21/2019 14:26:52	
CCB3	S	Reactive CN	P	0.7772	µg/l	1/21/2019 14:26:53	