

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

1/30/2019 13:47

Test: *Reactive* ~~Total~~ CN

Sample Id	Result <i>ug/d</i>	Dil. 1 +	Response	Errors
ICV1	97.169	0.0	0.091	
ICB1	-0.258	0.0	0.004	
CCV1	243.574	0.0	0.222	
CCB1	-0.287	0.0	0.004	
PB116720BL	-0.253	0.0	0.004	
K1271-01	-0.313	0.0	0.004	
K1271-01DUP	-0.439	0.0	0.004	
K1276-01	0.184	0.0	0.004	
K1282-04	-0.449	0.0	0.004	
K1282-08	-0.280	0.0	0.004	
K1282-12	-0.312	0.0	0.004	
K1282-16	-0.337	0.0	0.004	
K1282-20	-0.412	0.0	0.004	
K1282-24	-0.088	0.0	0.004	
CCV2	245.881	0.0	0.224	
CCB2	-0.349	0.0	0.004	
K1282-28	-0.514	0.0	0.004	
K1282-32	-0.156	0.0	0.004	
PB116721BL	-0.182	0.0	0.004	
K1277-04	-0.488	0.0	0.004	
K1282-36	-0.377	0.0	0.004	
K1277-04DUP	-0.440	0.0	0.004	
CCV3	264.562	0.0	0.241	
CCB3	-0.404	0.0	0.004	

N	24
Mean	35.210
SD	85.8385
CV%	243.79

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : As

1/30/2019 12:52


Test Total CN

Accepted 1/30/2019 12:52

Factor 1118
Bias 0.004

Coeff. of det. 0.999901

Errors

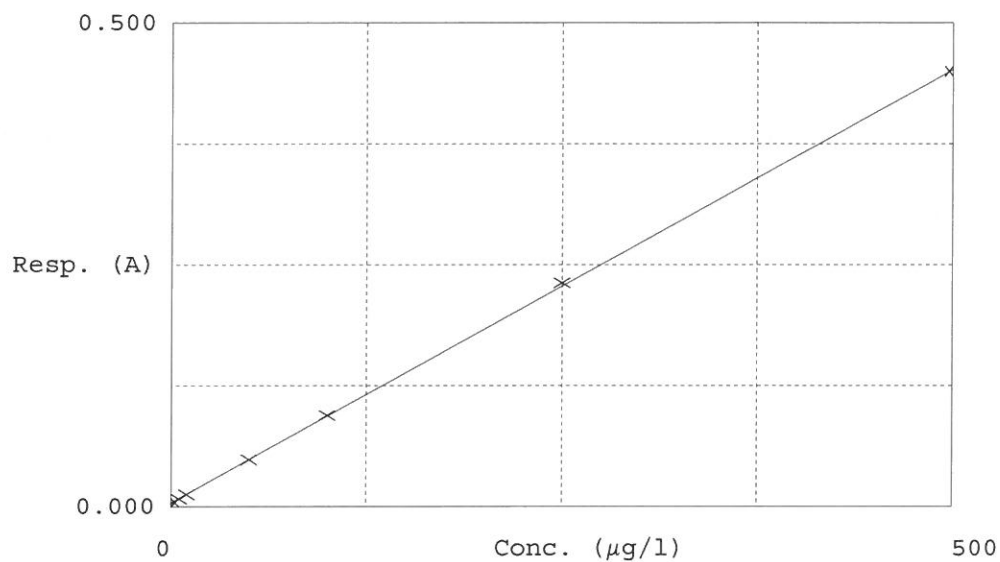

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.6793	0.0000	
2	5.0PPBCN	0.008	4.2319	5.0000	
3	10PPBCN	0.013	9.3220	10.0000	
4	50PPBCN	0.049	49.5733	50.0000	
5	100PPBCN	0.094	100.7592	100.0000	
6	250PPBCN	0.231	253.7617	250.0000	
7	500PPBCN	0.450	498.0312	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed Jan 30 12:44:52 2019

Wed Jan 30 13:47:13 2019

AS

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.6793	µg/l	1/30/2019 12:44:52	
5.OPPBCN	A	Reactive CN	P	4.2319	µg/l	1/30/2019 12:44:53	
10PPBCN	A	Reactive CN	P	9.322	µg/l	1/30/2019 12:44:54	
50PPBCN	A	Reactive CN	P	49.5733	µg/l	1/30/2019 12:44:55	
100PPBCN	A	Reactive CN	P	100.7592	µg/l	1/30/2019 12:44:56	
250PPBCN	A	Reactive CN	P	253.7617	µg/l	1/30/2019 12:44:57	
500PPBCN	A	Reactive CN	P	498.0312	µg/l	1/30/2019 12:44:58	
ICV1	S	Reactive CN	P	97.1687	µg/l	1/30/2019 13:19:46	
ICB1	S	Reactive CN	P	-0.2584	µg/l	1/30/2019 13:19:47	
CCV1	S	Reactive CN	P	243.5736	µg/l	1/30/2019 13:19:48	
CCB1	S	Reactive CN	P	-0.2867	µg/l	1/30/2019 13:19:49	
PB116720BL	S	Reactive CN	P	-0.2531	µg/l	1/30/2019 13:19:50	
K1271-01	S	Reactive CN	P	-0.3134	µg/l	1/30/2019 13:19:51	
K1271-01DUP	S	Reactive CN	P	-0.4391	µg/l	1/30/2019 13:19:52	
K1276-01	S	Reactive CN	P	0.1839	µg/l	1/30/2019 13:19:53	
K1282-04	S	Reactive CN	P	-0.4486	µg/l	1/30/2019 13:19:54	
K1282-08	S	Reactive CN	P	-0.2799	µg/l	1/30/2019 13:19:55	
K1282-12	S	Reactive CN	P	-0.312	µg/l	1/30/2019 13:19:56	
K1282-16	S	Reactive CN	P	-0.337	µg/l	1/30/2019 13:27:21	
K1282-20	S	Reactive CN	P	-0.4116	µg/l	1/30/2019 13:27:22	
K1282-24	S	Reactive CN	P	-0.0881	µg/l	1/30/2019 13:27:23	
CCV2	S	Reactive CN	P	245.881	µg/l	1/30/2019 13:27:24	
CCB2	S	Reactive CN	P	-0.3489	µg/l	1/30/2019 13:27:25	
K1282-28	S	Reactive CN	P	-0.5139	µg/l	1/30/2019 13:27:26	
K1282-32	S	Reactive CN	P	-0.1557	µg/l	1/30/2019 13:27:27	
PB116721BL	S	Reactive CN	P	-0.1819	µg/l	1/30/2019 13:27:28	
K1277-04	S	Reactive CN	P	-0.4884	µg/l	1/30/2019 13:27:29	
K1282-36	S	Reactive CN	P	-0.3772	µg/l	1/30/2019 13:27:31	
K1277-04DUP	S	Reactive CN	P	-0.4401	µg/l	1/30/2019 13:47:11	
CCV3	S	Reactive CN	P	264.5623	µg/l	1/30/2019 13:47:12	
CCB3	S	Reactive CN	P	-0.4035	µg/l	1/30/2019 13:47:13	