

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

2/21/2019 13:09

Test: ^{Reactive}~~Total~~ CN

Sample Id	Result ^{ug/d}	Dil. 1 +	Response	Errors
ICV1	96.239	0.0	0.090	
ICB1	-0.399	0.0	0.004	
CCV1	237.366	0.0	0.215	
CCB1	0.054	0.0	0.004	
PB117275BL	0.167	0.0	0.004	
K1344-02DUP	-0.182	0.0	0.004	
K1344-04	-0.180	0.0	0.004	
K1344-06	0.054	0.0	0.004	
K1344-08	0.160	0.0	0.004	
K1345-04	-0.032	0.0	0.004	
K1536-01	-0.215	0.0	0.004	
K1537-04	0.073	0.0	0.004	
K1538-04	0.217	0.0	0.004	
CCV2	238.542	0.0	0.216	
CCB2	0.282	0.0	0.004	
K1538-08	0.049	0.0	0.004	
K1546-03	0.235	0.0	0.004	
K1546-06	0.025	0.0	0.004	
K1546-09	0.095	0.0	0.004	
K1546-12	0.288	0.0	0.004	
K1546-15	0.192	0.0	0.004	
K1547-04	-0.159	0.0	0.004	
PB117276BL	-0.105	0.0	0.004	
K1549-04	-0.286	0.0	0.004	
K1549-04DUP	-0.132	0.0	0.004	
CCV3	243.347	0.0	0.221	
CCB3	0.045	0.0	0.004	
K1550-03	0.233	0.0	0.004	
K1344-02	0.108	0.0	0.004	
CCV4	255.527	0.0	0.231	
CCB4	-0.038	0.0	0.004	

N	31
Mean	34.567
SD	83.6617
CV%	242.03

Aquakem v. 7.2AQ1

Results from time period:

Thu Feb 21 12:11:03 2019

Thu Feb 21 13:08:23 2019



Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.0205	µg/l	2/21/2019 12:11:03	
5.OPPBCN	A	Reactive CN	P	4.8019	µg/l	2/21/2019 12:11:04	
10PPBCN	A	Reactive CN	P	10.7858	µg/l	2/21/2019 12:11:05	
50PPBCN	A	Reactive CN	P	50.2083	µg/l	2/21/2019 12:11:06	
100PPBCN	A	Reactive CN	P	100.6395	µg/l	2/21/2019 12:11:07	
250PPBCN	A	Reactive CN	P	247.4949	µg/l	2/21/2019 12:11:08	
500PPBCN	A	Reactive CN	P	501.0901	µg/l	2/21/2019 12:11:09	
ICV1	S	Reactive CN	P	96.2385	µg/l	2/21/2019 12:37:15	
ICB1	S	Reactive CN	P	-0.3985	µg/l	2/21/2019 12:37:16	
CCV1	S	Reactive CN	P	237.3656	µg/l	2/21/2019 12:37:17	
CCB1	S	Reactive CN	P	0.0542	µg/l	2/21/2019 12:37:18	
PB117275BL	S	Reactive CN	P	0.1669	µg/l	2/21/2019 12:37:19	
K1344-02DUP	S	Reactive CN	P	-0.1818	µg/l	2/21/2019 12:37:21	
K1344-04	S	Reactive CN	P	-0.1801	µg/l	2/21/2019 12:37:22	
K1344-06	S	Reactive CN	P	0.0542	µg/l	2/21/2019 12:37:23	
K1344-08	S	Reactive CN	P	0.1602	µg/l	2/21/2019 12:37:24	
K1345-04	S	Reactive CN	P	-0.0319	µg/l	2/21/2019 12:37:25	
K1536-01	S	Reactive CN	P	-0.215	µg/l	2/21/2019 12:44:47	
K1537-04	S	Reactive CN	P	0.0727	µg/l	2/21/2019 12:44:48	
K1538-04	S	Reactive CN	P	0.2165	µg/l	2/21/2019 12:44:49	
CCV2	S	Reactive CN	P	238.5419	µg/l	2/21/2019 12:44:50	
CCB2	S	Reactive CN	P	0.2817	µg/l	2/21/2019 12:44:51	
K1538-08	S	Reactive CN	P	0.0488	µg/l	2/21/2019 12:44:52	
K1546-03	S	Reactive CN	P	0.2353	µg/l	2/21/2019 12:44:53	
K1546-06	S	Reactive CN	P	0.0255	µg/l	2/21/2019 12:44:54	
K1546-09	S	Reactive CN	P	0.0954	µg/l	2/21/2019 12:44:55	
K1546-12	S	Reactive CN	P	0.2882	µg/l	2/21/2019 12:44:56	
K1546-15	S	Reactive CN	P	0.1916	µg/l	2/21/2019 12:44:57	
K1547-04	S	Reactive CN	P	-0.1593	µg/l	2/21/2019 12:51:26	
PB117276BL	S	Reactive CN	P	-0.1049	µg/l	2/21/2019 12:51:27	
K1549-04	S	Reactive CN	P	-0.2862	µg/l	2/21/2019 12:51:28	
K1549-04DUP	S	Reactive CN	P	-0.1322	µg/l	2/21/2019 12:51:29	
CCV3	S	Reactive CN	P	243.3467	µg/l	2/21/2019 12:51:30	
CCB3	S	Reactive CN	P	0.0454	µg/l	2/21/2019 12:51:31	
K1550-03	S	Reactive CN	P	0.2328	µg/l	2/21/2019 12:51:32	
K1344-02	S	Reactive CN	P	0.1082	µg/l	2/21/2019 13:08:21	
CCV4	S	Reactive CN	P	255.5272	µg/l	2/21/2019 13:08:22	
CCB4	S	Reactive CN	P	-0.0384	µg/l	2/21/2019 13:08:23	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

2/21/2019 12:11


Test Total CN

Accepted 2/21/2019 12:11

Factor 1123
Bias 0.004

Coeff. of det. 0.999958

Errors

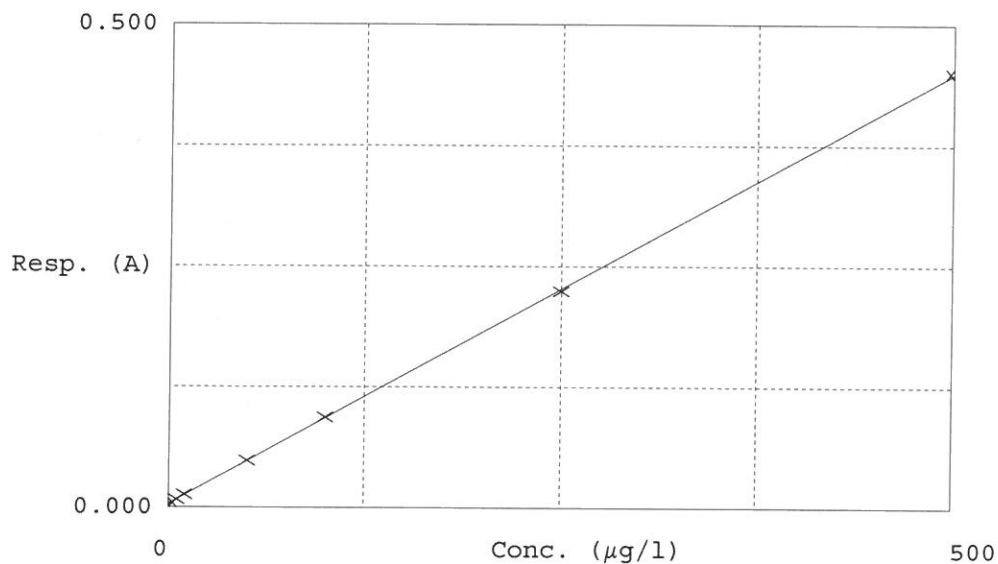

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.0205	0.0000	
2	5.0PPBCN	0.008	4.8019	5.0000	
3	10PPBCN	0.013	10.7858	10.0000	
4	50PPBCN	0.049	50.2083	50.0000	
5	100PPBCN	0.094	100.6395	100.0000	
6	250PPBCN	0.224	247.4949	250.0000	
7	500PPBCN	0.450	501.0901	500.0000	