

===== 2/10/007 =====
Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

2/25/2019 15:03

Test: Total CN

Sample Id	Result <i>ug/d</i>	Dil. 1 +	Response	Errors
ICV1	97.747	0.0	0.093	
ICB1	-0.360	0.0	0.004	
CCV1	245.532	0.0	0.226	
CCB1	-0.542	0.0	0.004	
PB117316BL	-0.475	0.0	0.004	
PB117316BS	98.688	0.0	0.094	
MIDPB117316	248.518	0.0	0.229	
K1560-10	2.897	0.0	0.007	
K1560-11	9.859	0.0	0.013	
CCV2	263.254	0.0	0.242	
CCB2	-0.800	0.0	0.004	

N	11
Mean	87.665
SD	112.3447
CV%	128.15

AS

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 25 14:50:32 2019

Mon Feb 25 14:53:56 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.7519	µg/l	2/25/2019 12:52:56	
5.OPPBCN	A	Total CN	P	4.3801	µg/l	2/25/2019 12:52:57	
10PPBCN	A	Total CN	P	9.7039	µg/l	2/25/2019 12:52:58	
50PPBCN	A	Total CN	P	50.2062	µg/l	2/25/2019 12:52:59	
100PPBCN	A	Total CN	P	100.4206	µg/l	2/25/2019 12:53:00	
250PPBCN	A	Total CN	P	252.2675	µg/l	2/25/2019 12:53:01	
500PPBCN	A	Total CN	P	498.7736	µg/l	2/25/2019 12:53:02	
ICV1	S	Total CN	P	97.747	µg/l	2/25/2019 14:50:32	
ICB1	S	Total CN	P	-0.3603	µg/l	2/25/2019 14:50:33	
CCV1	S	Total CN	P	245.5317	µg/l	2/25/2019 14:50:34	
CCB1	S	Total CN	P	-0.5416	µg/l	2/25/2019 14:50:35	
PB117316BL	S	Total CN	P	-0.4749	µg/l	2/25/2019 14:50:36	
PB117316BS	S	Total CN	P	98.688	µg/l	2/25/2019 14:50:37	
MIDPB117316	S	Total CN	P	248.5184	µg/l	2/25/2019 14:50:38	
K1560-10	S	Total CN	P	2.8968	µg/l	2/25/2019 14:50:40	
K1560-11	S	Total CN	P	9.8586	µg/l	2/25/2019 14:50:42	
CCV2	S	Total CN	P	263.254	µg/l	2/25/2019 14:53:55	
CCB2	S	Total CN	P	-0.7998	µg/l	2/25/2019 14:53:56	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

2/25/2019 12:54


Test Total CN

Accepted 2/25/2019 12:54

Factor 1105
Bias 0.004

Coeff. of det. 0.999962

Errors

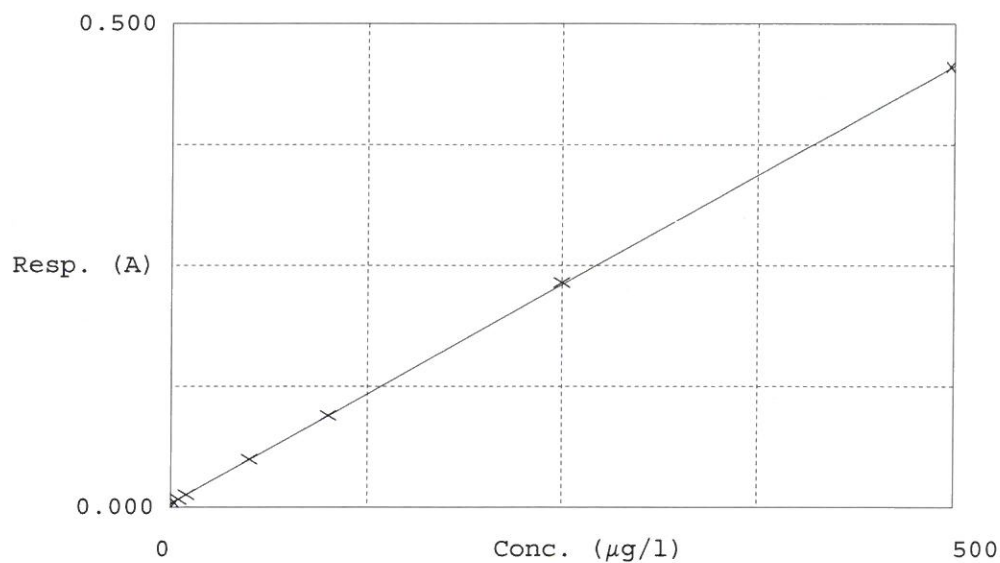

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.7519	0.0000	
2	5.0PPBCN	0.008	4.3801	5.0000	
3	10PPBCN	0.013	9.7039	10.0000	
4	50PPBCN	0.050	50.2062	50.0000	
5	100PPBCN	0.095	100.4206	100.0000	
6	250PPBCN	0.233	252.2675	250.0000	
7	500PPBCN	0.456	498.7736	500.0000	