

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/6/2019 12:28

Test: Nitrite

Sample Id	Result ^{mg/d}	Dil. 1 +	Response	Errors
ICV1	0.312	0.0	0.792	
ICB1	-0.003	0.0	0.006	Blank resp. low
CCV1	0.309	0.0	0.784	
CCB1	-0.003	0.0	0.007	Blank resp. low
LB101184BL	-0.003	0.0	0.006	
LB101184BS	0.310	0.0	0.787	
K1560-09	0.002	0.0	0.019	Blank resp. low
CCV2	0.311	0.0	0.791	
CCB2	-0.002	0.0	0.007	

N 9
Mean 0.137
SD 0.1645
CV% 120.03

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/6/2019 12:05


Test Nitrite

Accepted 3/6/2019 12:05

Factor 0.400
Bias 0.013

Coeff. of det. 0.999797

Errors Meas. error

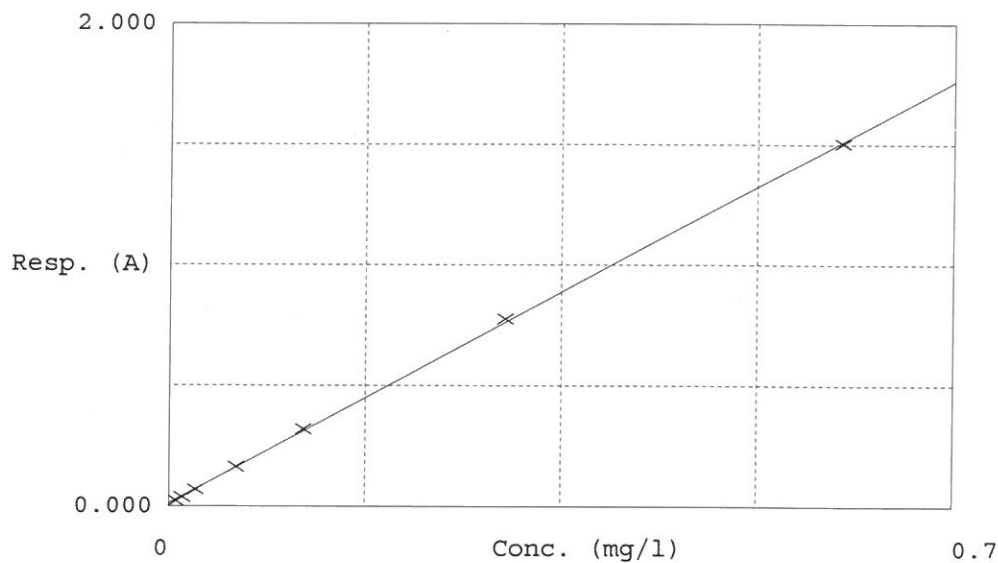

	Calibrator	Response	Calc. con.	Conc.	Errors
1	NITRITE0.6	0.022	0.0038	0.0060	Blank resp. low
2	NITRITE0.6	0.038	0.0101	0.0120	Blank resp. low
3	NITRITE0.6	0.069	0.0226	0.0240	Blank resp. low
4	NITRITE0.6	0.164	0.0604	0.0600	
5	NITRITE0.6	0.320	0.1229	0.1200	Blank resp. low
6	NITRITE0.6	0.776	0.3054	0.3000	Blank resp. low
7	NITRITE0.6	1.504	0.5968	0.6000	Blank resp. low

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 06 11:21:55 2019

Wed Mar 06 12:25:19 2019

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.0061PPM	A	Nitrite+Nitrate	P	0.0038	mg/l	3/6/2019 11:55:17	
0.0122PPM	A	Nitrite+Nitrate	P	0.0101	mg/l	3/6/2019 11:55:18	
0.0243PPM	A	Nitrite+Nitrate	P	0.0226	mg/l	3/6/2019 11:55:19	
0.0608PPM	A	Nitrite+Nitrate	P	0.0604	mg/l	3/6/2019 11:55:20	
0.1216PPM	A	Nitrite+Nitrate	P	0.1229	mg/l	3/6/2019 11:55:21	
0.304PPM	A	Nitrite+Nitrate	P	0.3054	mg/l	3/6/2019 11:55:22	
0.608PPM	A	Nitrite+Nitrate	P	0.5968	mg/l	3/6/2019 11:55:23	
ICV1	S	Nitrite+Nitrate	P	0.3119	mg/l	3/6/2019 12:25:10	
ICB1	S	Nitrite+Nitrate	P	-0.0029	mg/l	3/6/2019 12:25:11	
CCV1	S	Nitrite+Nitrate	P	0.3087	mg/l	3/6/2019 12:25:12	
CCB1	S	Nitrite+Nitrate	P	-0.0026	mg/l	3/6/2019 12:25:13	
LB101184BL	S	Nitrite+Nitrate	P	-0.0028	mg/l	3/6/2019 12:25:14	
LB101184BS	S	Nitrite+Nitrate	P	0.31	mg/l	3/6/2019 12:25:15	
K1560-09	S	Nitrite+Nitrate	P	0.0024	mg/l	3/6/2019 12:25:17	
CCV2	S	Nitrite+Nitrate	P	0.3113	mg/l	3/6/2019 12:25:18	
CCB2	S	Nitrite+Nitrate	P	-0.0024	mg/l	3/6/2019 12:25:19	