

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/6/2019 14:49

Test: Total CN

ug/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.562	0.0	0.093	
ICB1	-0.113	0.0	0.004	
CCV1	237.817	0.0	0.227	
CCB1	-0.287	0.0	0.004	
PB117667BL	-0.422	0.0	0.004	
K1753-04	-0.088	0.0	0.004	
K1753-04DUP	-0.680	0.0	0.004	
K1753-08	-0.562	0.0	0.004	
K1753-12	-0.253	0.0	0.004	
CCV2	239.904	0.0	0.229	
CCB2	-0.547	0.0	0.004	

N	11
Mean	51.757
SD	96.7404
CV%	186.91

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 06 14:48:40 2019

Wed Mar 06 14:48:50 2019

AS

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.3772	µg/l	3/6/2019 13:20:34	
5.0PPBCN	A	Reactive CN	P	4.4317	µg/l	3/6/2019 13:20:35	
10PPBCN	A	Reactive CN	P	9.6091	µg/l	3/6/2019 13:20:36	
50PPBCN	A	Reactive CN	P	49.9046	µg/l	3/6/2019 13:20:37	
100PPBCN	A	Reactive CN	P	101.0139	µg/l	3/6/2019 13:20:38	
250PPBCN	A	Reactive CN	P	251.1953	µg/l	3/6/2019 13:20:39	
500PPBCN	A	Reactive CN	P	499.2226	µg/l	3/6/2019 13:20:40	
ICV1	S	Reactive CN	P	94.5617	µg/l	3/6/2019 14:48:40	
ICB1	S	Reactive CN	P	-0.1131	µg/l	3/6/2019 14:48:41	
CCV1	S	Reactive CN	P	237.8166	µg/l	3/6/2019 14:48:42	
CCB1	S	Reactive CN	P	-0.287	µg/l	3/6/2019 14:48:43	
PB117667BL	S	Reactive CN	P	-0.4215	µg/l	3/6/2019 14:48:44	
K1753-04	S	Reactive CN	P	-0.088	µg/l	3/6/2019 14:48:45	
K1753-04DUP	S	Reactive CN	P	-0.6803	µg/l	3/6/2019 14:48:46	
K1753-08	S	Reactive CN	P	-0.5616	µg/l	3/6/2019 14:48:47	
K1753-12	S	Reactive CN	P	-0.2527	µg/l	3/6/2019 14:48:48	
CCV2	S	Reactive CN	P	239.9043	µg/l	3/6/2019 14:48:49	
CCB2	S	Reactive CN	P	-0.5474	µg/l	3/6/2019 14:48:50	

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/6/2019 13:24


Test Total CN

Accepted 3/6/2019 13:24

Factor 1070
Bias 0.004

Coeff. of det. 0.999982

Errors

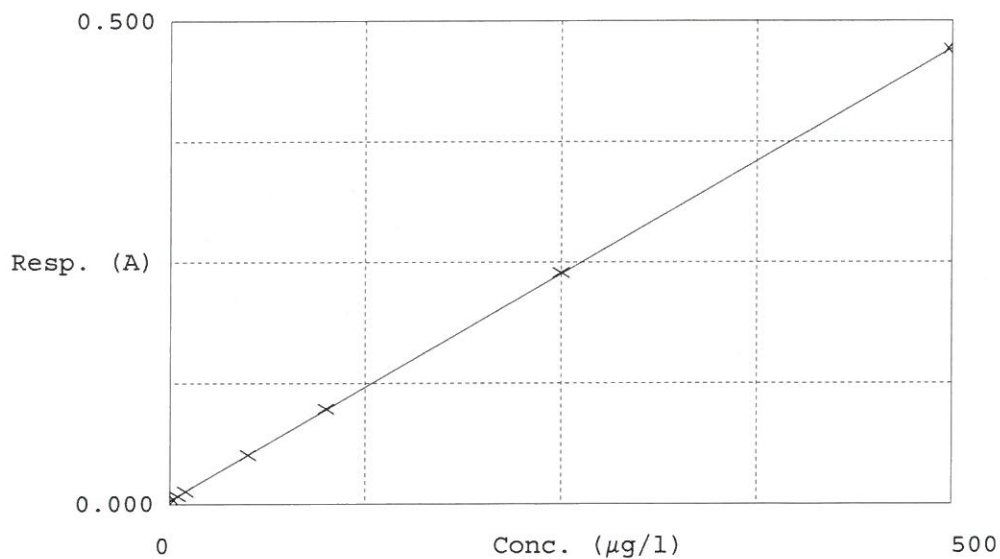

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.3772	0.0000	
2	5.0PPBCN	0.008	4.4317	5.0000	
3	10PPBCN	0.013	9.6091	10.0000	
4	50PPBCN	0.051	49.9046	50.0000	
5	100PPBCN	0.099	101.0139	100.0000	
6	250PPBCN	0.239	251.1953	250.0000	
7	500PPBCN	0.471	499.2226	500.0000	