

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/20/2019 15:18

Test: *Positive*
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.426	0.0	0.096	
ICB1	0.301	0.0	0.004	
CCV1	240.871	0.0	0.235	
CCB1	-0.127	0.0	0.004	
PB118097BL	0.094	0.0	0.004	
K1688-22	0.001	0.0	0.004	
K1688-22DUP	-0.165	0.0	0.004	
K1688-24	-0.103	0.0	0.004	
K1688-26	-0.131	0.0	0.004	
K1688-28	0.140	0.0	0.004	
K1688-30	-0.247	0.0	0.004	
K1688-32	0.101	0.0	0.004	
K1688-34	0.088	0.0	0.004	
K1688-36	0.296	0.0	0.004	
CCV2	242.299	0.0	0.236	
CCB2	0.105	0.0	0.004	
K1688-38	0.182	0.0	0.004	
K1688-40	0.021	0.0	0.004	
K1984-03	0.006	0.0	0.004	
K1984-05	-0.119	0.0	0.004	
K1989-04	0.352	0.0	0.004	
K1994-01	-0.266	0.0	0.004	
K1994-02	-0.273	0.0	0.004	
K1994-03	-0.004	0.0	0.004	
K1994-05	-0.311	0.0	0.004	
CCV3	252.856	0.0	0.247	
CCB3	0.194	0.0	0.004	
PB118070BL	-0.098	0.0	0.004	
K1956-04	-0.180	0.0	0.004	
K1956-04DUP	-0.174	0.0	0.004	
K1956-08	0.093	0.0	0.004	
K1971-11	0.148	0.0	0.004	
CCV4	249.649	0.0	0.244	
CCB4	-0.200	0.0	0.004	

N	34
Mean	31.789
SD	81.2287
CV%	255.52

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/20/2019 15:24


Test Total CN

Accepted 3/20/2019 8:24

Factor 1043
Bias 0.004

Coeff. of det. 0.999979

Errors

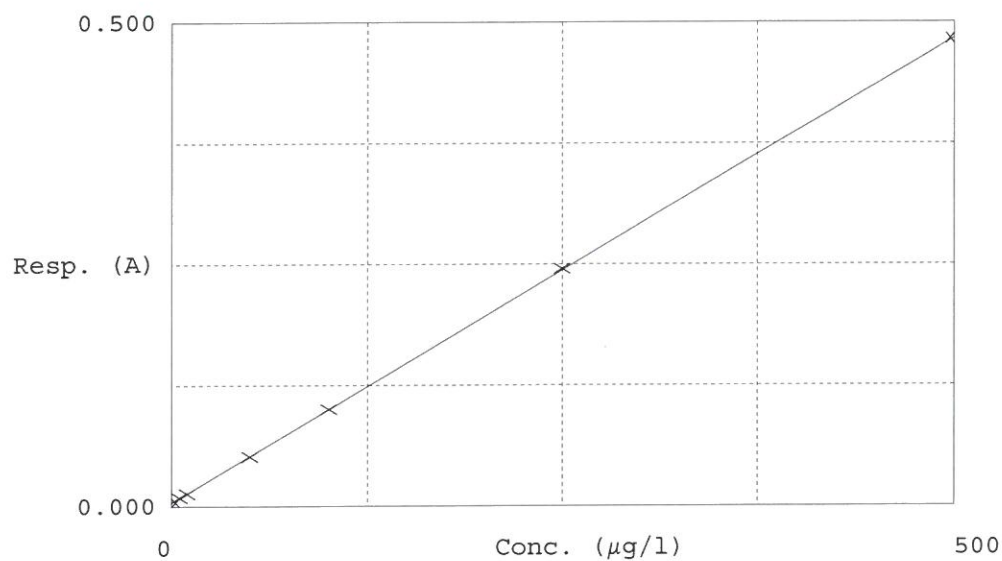

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.4305	0.0000	
2	5.0PPBCN	0.009	5.4117	5.0000	
3	10PPBCN	0.013	9.4860	10.0000	
4	50PPBCN	0.052	49.4950	50.0000	
5	100PPBCN	0.100	100.2060	100.0000	
6	250PPBCN	0.245	251.6330	250.0000	
7	500PPBCN	0.483	499.1990	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 20 13:59:44 2019

Wed Mar 20 14:53:30 2019

حضر

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.4305	µg/l	3/20/2019 8:23:07	
5.OPPBCN	A	Reactive CN	P	5.4117	µg/l	3/20/2019 8:23:08	
10PPBCN	A	Reactive CN	P	9.486	µg/l	3/20/2019 8:23:09	
50PPBCN	A	Reactive CN	P	49.495	µg/l	3/20/2019 8:23:10	
100PPBCN	A	Reactive CN	P	100.206	µg/l	3/20/2019 8:23:11	
250PPBCN	A	Reactive CN	P	251.633	µg/l	3/20/2019 8:23:12	
500PPBCN	A	Reactive CN	P	499.199	µg/l	3/20/2019 8:23:13	
ICV1	S	Reactive CN	P	95.4256	µg/l	3/20/2019 13:59:44	
ICB1	S	Reactive CN	P	0.3012	µg/l	3/20/2019 13:59:45	
CCV1	S	Reactive CN	P	240.8705	µg/l	3/20/2019 13:59:46	
CCB1	S	Reactive CN	P	-0.1267	µg/l	3/20/2019 13:59:47	
PB118097BL	S	Reactive CN	P	0.0941	µg/l	3/20/2019 13:59:48	
K1688-22	S	Reactive CN	P	0.0012	µg/l	3/20/2019 13:59:49	
K1688-22DUP	S	Reactive CN	P	-0.1653	µg/l	3/20/2019 13:59:50	
K1688-24	S	Reactive CN	P	-0.1031	µg/l	3/20/2019 13:59:51	
K1688-26	S	Reactive CN	P	-0.1307	µg/l	3/20/2019 13:59:52	
K1688-28	S	Reactive CN	P	0.14	µg/l	3/20/2019 13:59:53	
K1688-30	S	Reactive CN	P	-0.2467	µg/l	3/20/2019 13:59:54	
K1688-32	S	Reactive CN	P	0.101	µg/l	3/20/2019 14:07:19	
K1688-34	S	Reactive CN	P	0.0884	µg/l	3/20/2019 14:07:20	
K1688-36	S	Reactive CN	P	0.2964	µg/l	3/20/2019 14:07:21	
CCV2	S	Reactive CN	P	242.2993	µg/l	3/20/2019 14:07:22	
CCB2	S	Reactive CN	P	0.1054	µg/l	3/20/2019 14:07:23	
K1688-38	S	Reactive CN	P	0.182	µg/l	3/20/2019 14:07:24	
K1688-40	S	Reactive CN	P	0.0213	µg/l	3/20/2019 14:07:25	
K1984-03	S	Reactive CN	P	0.0057	µg/l	3/20/2019 14:07:26	
K1984-05	S	Reactive CN	P	-0.1194	µg/l	3/20/2019 14:07:27	
K1989-04	S	Reactive CN	P	0.3519	µg/l	3/20/2019 14:07:28	
K1994-01	S	Reactive CN	P	-0.2659	µg/l	3/20/2019 14:07:29	
K1994-02	S	Reactive CN	P	-0.2731	µg/l	3/20/2019 14:12:06	
K1994-03	S	Reactive CN	P	-0.0036	µg/l	3/20/2019 14:12:07	
K1994-05	S	Reactive CN	P	-0.3107	µg/l	3/20/2019 14:12:08	
CCV3	S	Reactive CN	P	252.8563	µg/l	3/20/2019 14:12:09	
CCB3	S	Reactive CN	P	0.1945	µg/l	3/20/2019 14:12:10	
PB118070BL	S	Reactive CN	P	-0.0984	µg/l	3/20/2019 14:53:24	
K1956-04	S	Reactive CN	P	-0.18	µg/l	3/20/2019 14:53:25	
K1956-04DUP	S	Reactive CN	P	-0.1737	µg/l	3/20/2019 14:53:26	
K1956-08	S	Reactive CN	P	0.0926	µg/l	3/20/2019 14:53:27	
K1971-11	S	Reactive CN	P	0.1478	µg/l	3/20/2019 14:53:28	
CCV4	S	Reactive CN	P	249.6493	µg/l	3/20/2019 14:53:29	
CCB4	S	Reactive CN	P	-0.2004	µg/l	3/20/2019 14:53:30	