

2/13/017.52

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/29/2019 15:18

Test: Reactive
~~Total~~ CN

Sample Id	Result <u>mg/L</u>	Dil. 1 +	Response	Errors
ICV1	96.856	0.0	0.093	
ICB1	0.360	0.0	0.004	
CCV1	242.025	0.0	0.226	
CCB1	0.091	0.0	0.004	
PB118416BL	0.108	0.0	0.004	
K1685-10	0.147	0.0	0.004	
K1685-10DUP	-0.119	0.0	0.004	
K1685-12	-0.109	0.0	0.004	
K1685-14	-0.068	0.0	0.004	
K1698-04	0.010	0.0	0.004	
K2138-02	-0.138	0.0	0.004	
K2138-04	0.334	0.0	0.004	
K2138-06	0.357	0.0	0.004	
K2138-08	0.253	0.0	0.004	
CCV2	241.398	0.0	0.226	
CCB2	0.226	0.0	0.004	
K2138-10	0.552	0.0	0.004	
K2139-02	0.181	0.0	0.004	
K2139-04	0.078	0.0	0.004	
K2153-24	-0.123	0.0	0.004	
K2153-28	0.093	0.0	0.004	
CCV3	238.780	0.0	0.223	
CCB3	-0.200	0.0	0.004	

N	23
Mean	35.700
SD	83.6482
CV%	234.31

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/29/2019 15:18


Test Total CN

Accepted 3/29/2019 10:42

Factor 1089
Bias 0.004

Coeff. of det. 1.000000

Errors

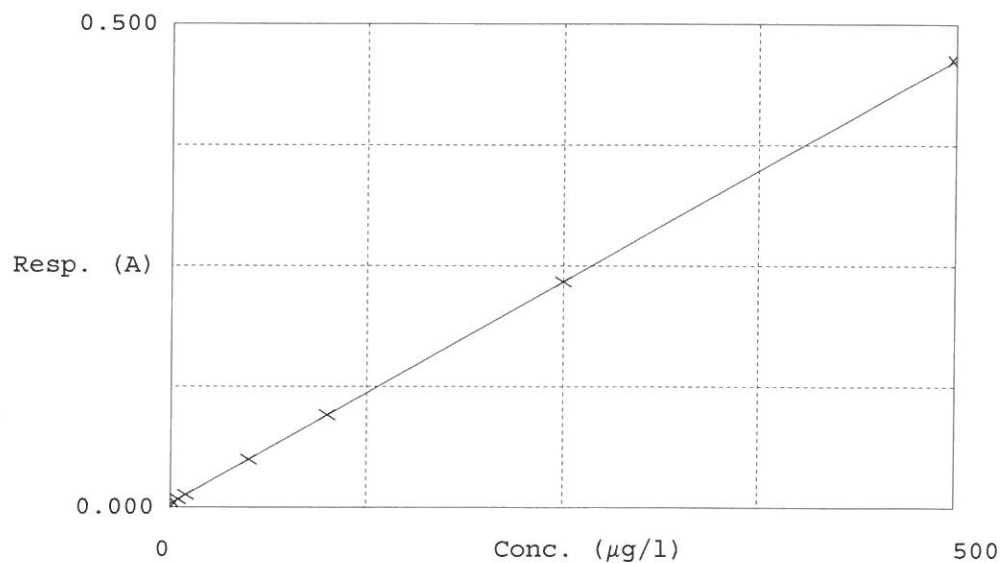

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.0054	0.0000	
2	5.0PPBCN	0.008	4.8446	5.0000	
3	10PPBCN	0.013	10.0190	10.0000	
4	50PPBCN	0.050	50.0326	50.0000	
5	100PPBCN	0.096	100.1689	100.0000	
6	250PPBCN	0.233	249.9307	250.0000	
7	500PPBCN	0.463	499.9988	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri Mar 29 14:18:37 2019

Fri Mar 29 14:29:36 2019

AS

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.0054	µg/l	3/29/2019 10:28:45	
5.0PPBCN	A	Reactive CN	P	4.8446	µg/l	3/29/2019 10:28:46	
10PPBCN	A	Reactive CN	P	10.019	µg/l	3/29/2019 10:28:47	
50PPBCN	A	Reactive CN	P	50.0326	µg/l	3/29/2019 10:28:48	
100PPBCN	A	Reactive CN	P	100.1689	µg/l	3/29/2019 10:28:49	
250PPBCN	A	Reactive CN	P	249.9307	µg/l	3/29/2019 10:28:50	
500PPBCN	A	Reactive CN	P	499.9988	µg/l	3/29/2019 10:28:51	
ICV1	S	Reactive CN	P	96.8564	µg/l	3/29/2019 14:18:37	
ICB1	S	Reactive CN	P	0.3605	µg/l	3/29/2019 14:18:38	
CCV1	S	Reactive CN	P	242.0253	µg/l	3/29/2019 14:18:39	
CCB1	S	Reactive CN	P	0.091	µg/l	3/29/2019 14:18:40	
PB118416BL	S	Reactive CN	P	0.1085	µg/l	3/29/2019 14:18:41	
K1685-10	S	Reactive CN	P	0.1473	µg/l	3/29/2019 14:18:42	
K1685-10DUP	S	Reactive CN	P	-0.1188	µg/l	3/29/2019 14:18:43	
K1685-12	S	Reactive CN	P	-0.1089	µg/l	3/29/2019 14:18:44	
K1685-14	S	Reactive CN	P	-0.0678	µg/l	3/29/2019 14:18:45	
K1698-04	S	Reactive CN	P	0.01	µg/l	3/29/2019 14:18:46	
K2138-02	S	Reactive CN	P	-0.1383	µg/l	3/29/2019 14:18:47	
K2138-04	S	Reactive CN	P	0.334	µg/l	3/29/2019 14:26:12	
K2138-06	S	Reactive CN	P	0.3567	µg/l	3/29/2019 14:26:13	
K2138-08	S	Reactive CN	P	0.2533	µg/l	3/29/2019 14:26:14	
CCV2	S	Reactive CN	P	241.3978	µg/l	3/29/2019 14:26:15	
CCB2	S	Reactive CN	P	0.2257	µg/l	3/29/2019 14:26:16	
K2138-10	S	Reactive CN	P	0.5518	µg/l	3/29/2019 14:26:17	
K2139-02	S	Reactive CN	P	0.1812	µg/l	3/29/2019 14:26:18	
K2139-04	S	Reactive CN	P	0.0781	µg/l	3/29/2019 14:26:19	
K2153-24	S	Reactive CN	P	-0.1231	µg/l	3/29/2019 14:26:20	
K2153-28	S	Reactive CN	P	0.0929	µg/l	3/29/2019 14:26:21	
CCV3	S	Reactive CN	P	238.7799	µg/l	3/29/2019 14:26:22	
CCB3	S	Reactive CN	P	-0.2005	µg/l	3/29/2019 14:29:35	