

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/4/2019 14:38

Test: Reactive Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.085	0.0	0.092	
ICB1	-0.179	0.0	0.005	
CCV1	241.549	0.0	0.222	
CCB1	-0.428	0.0	0.004	
PB118622BL	-0.636	0.0	0.004	
K2193-02	-0.639	0.0	0.004	
K2193-02DUP	-0.724	0.0	0.004	
K2193-04	-0.776	0.0	0.004	
K2193-06	-0.832	0.0	0.004	
K2195-02	-0.663	0.0	0.004	
K2240-11	-0.883	0.0	0.004	
K2240-12	-0.523	0.0	0.004	
K2240-13	-0.539	0.0	0.004	
K2240-14	-0.693	0.0	0.004	
CCV2	240.067	0.0	0.221	
CCB2	-0.522	0.0	0.004	
K2240-15	-0.499	0.0	0.004	
K2240-16	-0.900	0.0	0.004	
K2240-17	-0.690	0.0	0.004	
K2240-18	-0.663	0.0	0.004	
K2240-19	-0.596	0.0	0.004	
K2245-04	-0.938	0.0	0.004	
K2245-08	-0.531	0.0	0.004	
K2245-12	-0.689	0.0	0.004	
K2245-16	-0.798	0.0	0.004	
K2258-03	-0.484	0.0	0.004	
CCV3	251.938	0.0	0.232	
CCB3	-0.547	0.0	0.004	

N	28
Mean	29.117
SD	78.2089
CV%	268.60

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

4/4/2019 13:05


Test Total CN

Accepted 4/4/2019 13:05

Factor 1110
Bias 0.005

Coeff. of det. 0.999957

Errors

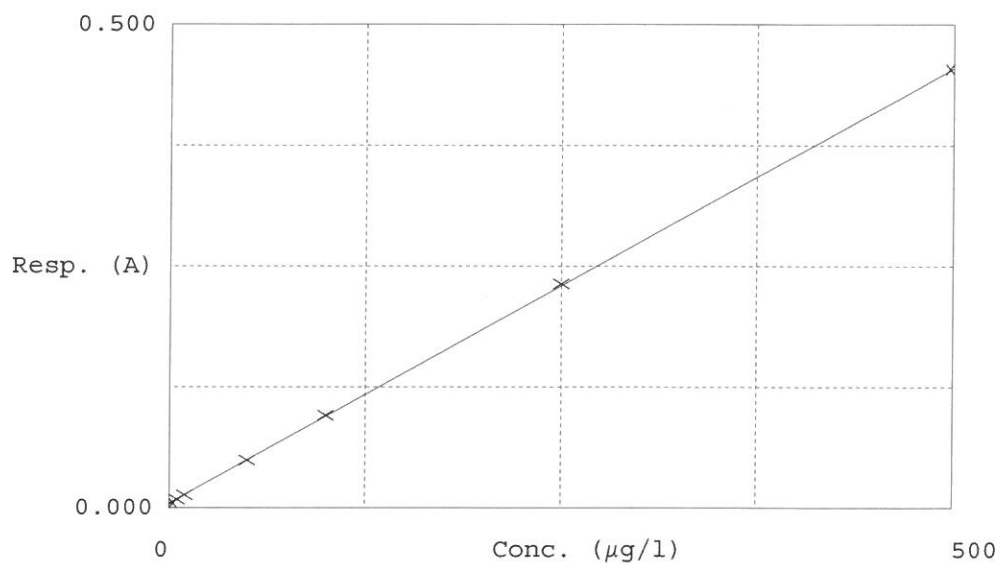

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.5738	0.0000	
2	5.0PPBCN	0.009	4.3871	5.0000	
3	10PPBCN	0.013	9.6076	10.0000	
4	50PPBCN	0.049	49.5053	50.0000	
5	100PPBCN	0.096	101.1327	100.0000	
6	250PPBCN	0.232	252.2084	250.0000	
7	500PPBCN	0.454	498.7327	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Apr 04 14:25:53 2019

Thu Apr 04 14:38:45 2019

AS

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.5738	µg/l	4/4/2019 13:03:12	
5.0PPBCN	A	Reactive CN	P	4.3871	µg/l	4/4/2019 13:03:13	
10PPBCN	A	Reactive CN	P	9.6076	µg/l	4/4/2019 13:03:14	
50PPBCN	A	Reactive CN	P	49.5053	µg/l	4/4/2019 13:03:15	
100PPBCN	A	Reactive CN	P	101.1327	µg/l	4/4/2019 13:03:16	
250PPBCN	A	Reactive CN	P	252.2084	µg/l	4/4/2019 13:03:17	
500PPBCN	A	Reactive CN	P	498.7327	µg/l	4/4/2019 13:03:18	
ICV1	S	Reactive CN	P	97.0846	µg/l	4/4/2019 14:25:53	
ICB1	S	Reactive CN	P	-0.1788	µg/l	4/4/2019 14:25:54	
CCV1	S	Reactive CN	P	241.5492	µg/l	4/4/2019 14:25:55	
CCB1	S	Reactive CN	P	-0.4277	µg/l	4/4/2019 14:25:56	
PB118622BL	S	Reactive CN	P	-0.6356	µg/l	4/4/2019 14:25:57	
K2193-02	S	Reactive CN	P	-0.6386	µg/l	4/4/2019 14:25:58	
K2193-02DUP	S	Reactive CN	P	-0.7245	µg/l	4/4/2019 14:25:59	
K2193-04	S	Reactive CN	P	-0.7762	µg/l	4/4/2019 14:26:00	
K2193-06	S	Reactive CN	P	-0.8317	µg/l	4/4/2019 14:26:01	
K2195-02	S	Reactive CN	P	-0.6632	µg/l	4/4/2019 14:26:02	
K2240-11	S	Reactive CN	P	-0.8831	µg/l	4/4/2019 14:26:03	
K2240-12	S	Reactive CN	P	-0.5228	µg/l	4/4/2019 14:33:25	
K2240-13	S	Reactive CN	P	-0.539	µg/l	4/4/2019 14:33:26	
K2240-14	S	Reactive CN	P	-0.6931	µg/l	4/4/2019 14:33:27	
CCV2	S	Reactive CN	P	240.0674	µg/l	4/4/2019 14:33:28	
CCB2	S	Reactive CN	P	-0.5221	µg/l	4/4/2019 14:33:29	
K2240-15	S	Reactive CN	P	-0.499	µg/l	4/4/2019 14:33:30	
K2240-16	S	Reactive CN	P	-0.8997	µg/l	4/4/2019 14:33:31	
K2240-17	S	Reactive CN	P	-0.6903	µg/l	4/4/2019 14:33:32	
K2240-18	S	Reactive CN	P	-0.6633	µg/l	4/4/2019 14:33:33	
K2240-19	S	Reactive CN	P	-0.5956	µg/l	4/4/2019 14:33:34	
K2245-04	S	Reactive CN	P	-0.9376	µg/l	4/4/2019 14:33:35	
K2245-08	S	Reactive CN	P	-0.5309	µg/l	4/4/2019 14:38:40	
K2245-12	S	Reactive CN	P	-0.6886	µg/l	4/4/2019 14:38:41	
K2245-16	S	Reactive CN	P	-0.7984	µg/l	4/4/2019 14:38:42	
K2258-03	S	Reactive CN	P	-0.4836	µg/l	4/4/2019 14:38:43	
CCV3	S	Reactive CN	P	251.9379	µg/l	4/4/2019 14:38:44	
CCB3	S	Reactive CN	P	-0.5474	µg/l	4/4/2019 14:38:45	